





Product name:	PageWriter Trim Cardiographs (Trim I)	
Identification code(s)	PW Trim I: 860290	
Total weight (in Kg)	7.0 Kg (Cardiograph w/battery and PIM), 1.2 Kg (Battery)	
Producer/ Manufacturer	Name company:	Philips Medical Systems
	Address:	3000 Minuteman Road, Andover Ma
	Zip code:	01810
	Country:	USA

Recycle Info	Items:	Location
Special attention 	First Steps: Disconnect power cord and remove battery before starting disassembly of the unit. Special Tools Needed: Torx 10 Driver to remove LCD display, Torx 6 for Keyboard and Torx 15 for Lower case. PW Trim Repair manual 453564010431 provides additional information for disassembly.	N/A

Fluids / Gases	Items:	Location
		N/A
	None	


Batteries	Type:	Location
	Lead (Pb) Acid Battery Philips Part # 989803130151	See page 4

Hazardous	Substances:	Location
	Liquid Crystal Display (LCD) with HG	See pages 2, 3
	Cardiograph has 4 circuit boards	Several locations inside the cardiograph And PIM
	Patient Interface Module (PIM) has 2 circuit boards	
	To be Removed	

Printed copies are uncontrolled


Show locations of materials mentioned on the previous sheet. (Picture information)

Figure 1-1 PageWriter Trim I Cardlograph and Cart (Front View)

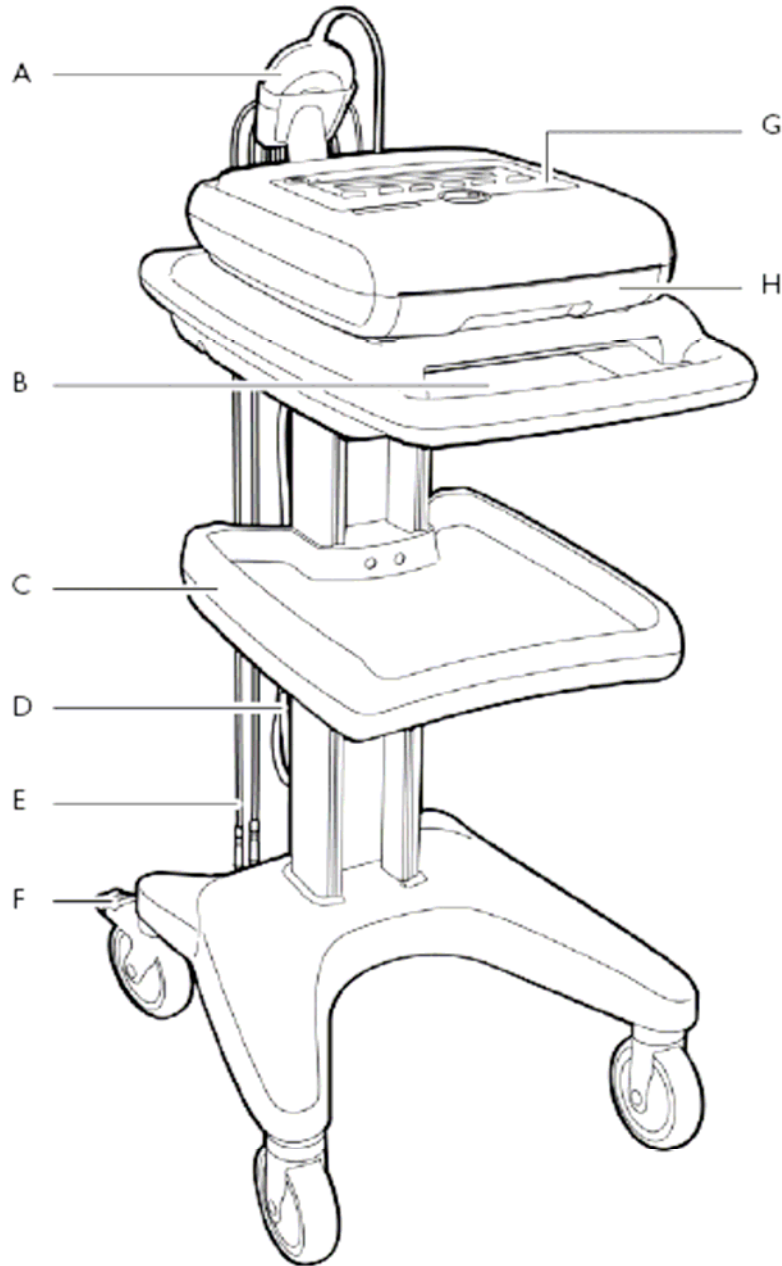

- A** Patient Interface Module (PIM)
- B** Printer paper/report storage slot
- C** Storage shelf
- D** AC Power cord

- E** PIM leads
- F** Wheel brake
- G** Control panel
- H** Printer paper drawer

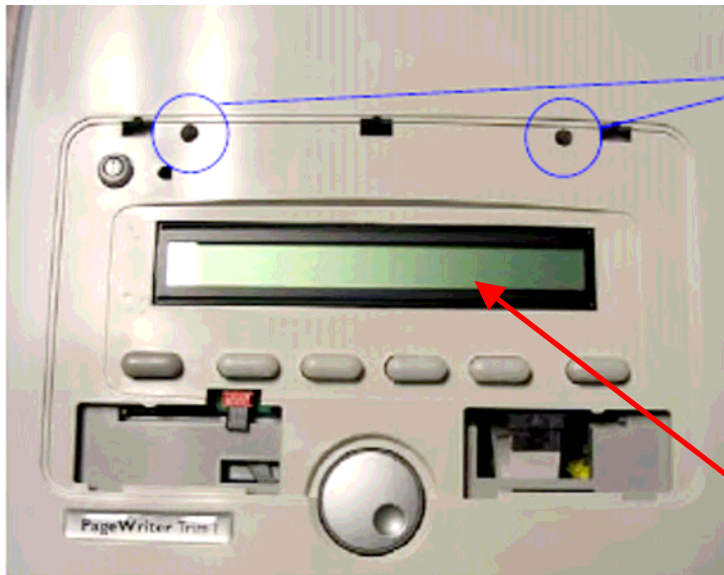


Front panel screws

Use Torx 10 driver to remove screws at top of LCD display assembly.



Printed copies are uncontrolled

Figure 1-2 PageWriter Trim I Cardlograph (Rear View)

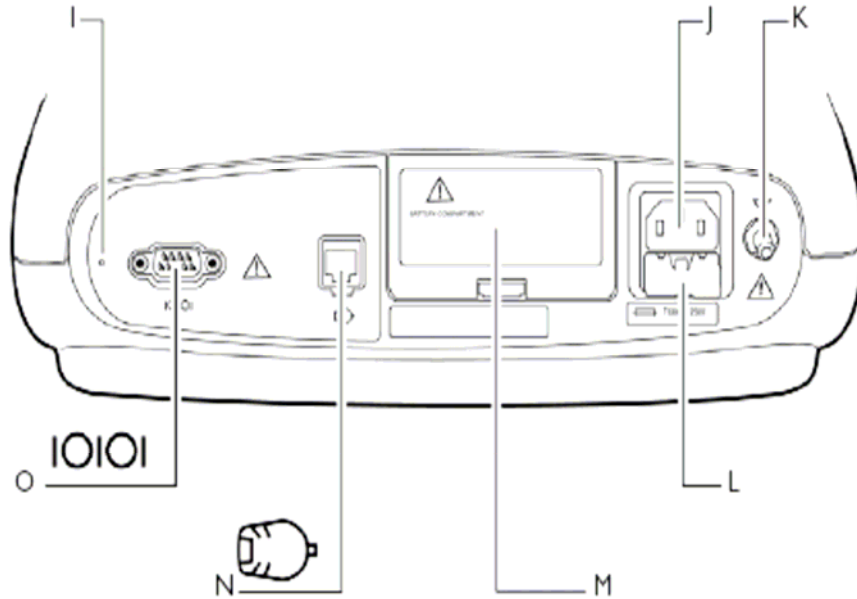

- I Reset button
- J AC power cord connector
- K Equipotential post
- L Fuse door
- M Battery door
- N PIM connector
- O Serial connector (not supported)

