





Recycling Passport

Product name:	Upgr.Dig.Diagnost 50kW/480V USA		
Identification code	9890-000-62103		
Order No.			
Device Type	B2B (Business to business)		
Producer /Manufacturer	Company name:	Philips Medical Systems DMC GmbH	
	Address:	Roentgenstrasse 24	
	Zip code:	22335 Hamburg	
	Country:	Germany	
	Web info:	http://www.medical.philips.com/main/company/sustainability/recycling/xray_generators/	
Total weight (in Kg) thereof			242

steel, iron	iron, low alloy (<5%)	106,268	KG
	iron, high alloy (>5%)	1,73	KG
steel, iron		107,998	KG
nonferrous metals and alloys	copper, -alloy	6,068	KG
	aluminum, -alloy	1,056	KG
	zinc, -alloy	0,438	KG
nonferrous metals and alloys		7,562	KG
glass / ceramics	glass	0,288	KG
	glass / ceramics		0,288
plastics / organic substances	lubricating grease	44,25	KG
	thermoplastic	5,999	KG
	thermoset	2,778	KG
	elastomer	0,205	KG
	oil	0,069	KG
plastics / organic substances		53,301	KG
standard parts	other electronic powered devices	49,757	KG
	cables	10,456	KG
	printed circuit boards	10,363	KG
	mounting parts, attaching part	2,52	KG
	motors, pumps	0,138	KG
	fans	0,064	KG
standard parts		73,298	KG
Not relevant for substances list	No relevant for subst. list		
Not relevant for substances list			
		242,447	KG

Recycling Passport

Recycle info		
General Hazards (Desinfection)	For dismantling activities Treatment Facilities must consider the national requirements. For personnel which can come into contact with contaminated material, preventive measures pursuant to national requirements must be taken into account	
Hazardous Substances  To be removed	Substances:	Location
Batteries  To be removed	Type:	Location
	Lithium chrome cell, 3V	Figure 1 (1)
	Lithium chrome cell, 3V	Figure 1 (2)
Special attention 	Item	Location
	Pb is present in the soldering process of PCBs	Figure 1, 2
Fluids / Gases 	Item	Location
	Transformer Oil, Shell Diala	Figure 1 (3)
	HV-transformer oil contains no PCBs	

Recycling Passport

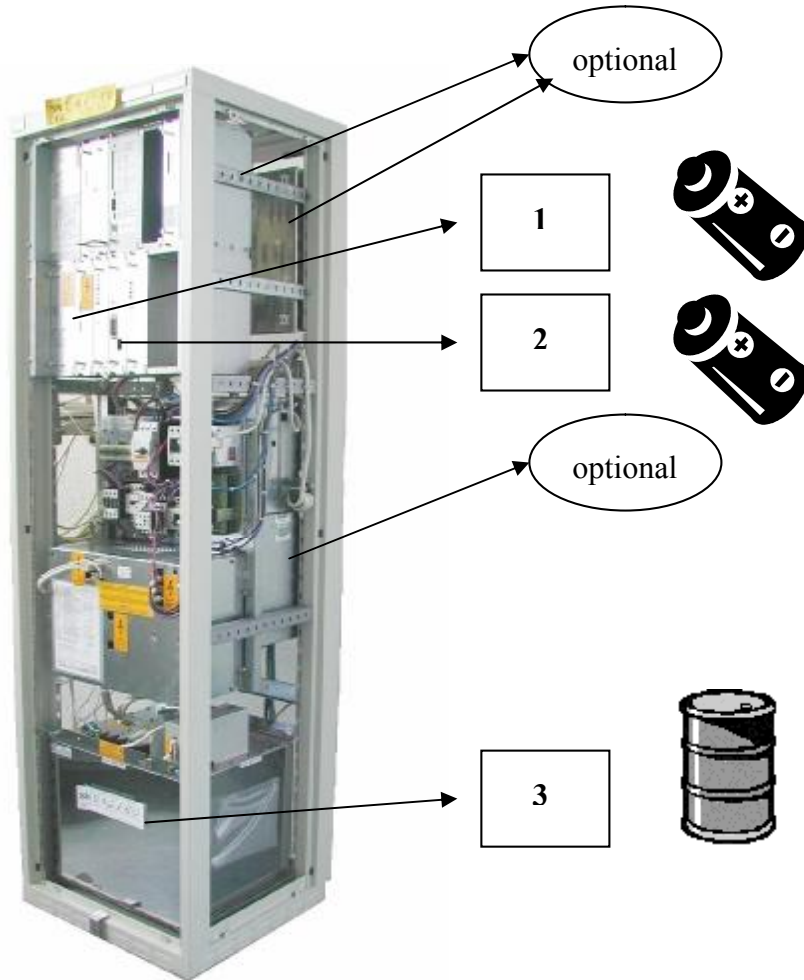


Figure 1



Figure 2