


---

# DICOM

## Conformance Statement

### GEMINI TF Version 3.1

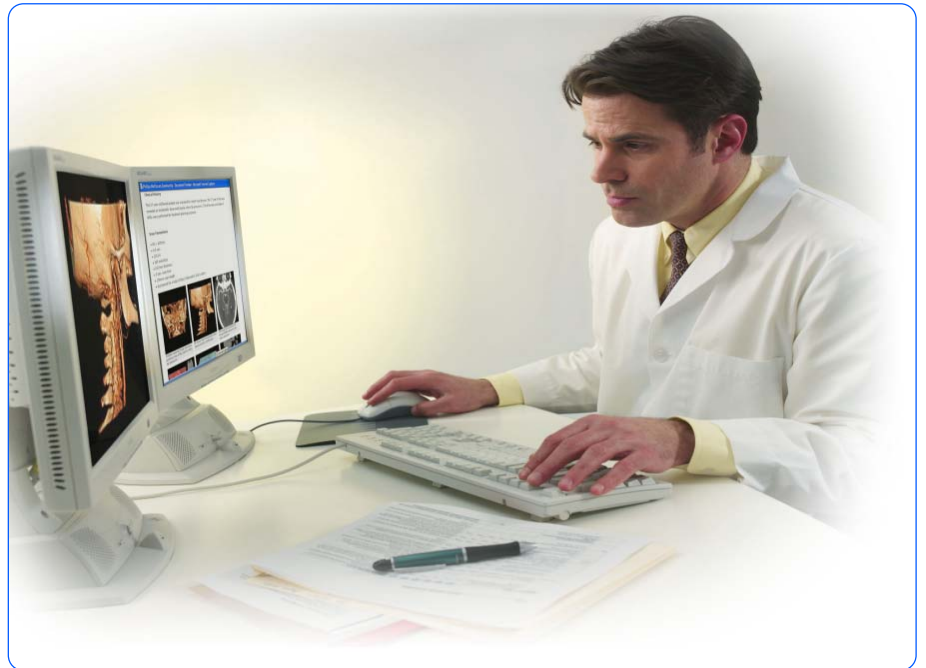

***Issued by:***

Philips Medical Systems (Cleveland), Inc.  
Philips Medical Systems  
595 Miner Road  
Cleveland, Ohio 44143  
USA

**Philips Medical Systems Nederland B.V.  
Medical IT, Interoperability**

**Building QV-282  
P.O. Box 10.000  
5680 DA Best  
The Netherlands**

email: <mailto:dicom@philips.com>  
Internet: <http://www.medical.philips.com>

Document Number: 4535 679 94381 Rev. B  
Date: August 18, 2006

## 1. DICOM CONFORMANCE STATEMENT OVERVIEW

This conformance statement refers to the GEMINI TF PET/CT Imaging System running PET software version 9.2 and CT Brilliance 3.01 on the PET/CT Host.

The first column specifies the used SOP classes exactly as named in PS 3.6. (Ref. PS 3.2 Annex A.) of the DICOM Standard.

**Table 1: Network Services**

SOP Class		User of Service (SCU)	Provider of Service (SCP)
Name	UID		
<b>Transfer</b>			
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	Yes	Yes
Digital X-Ray Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.1	Yes	Yes
Digital X-Ray Image Storage – for Processing	1.2.840.10008.5.1.4.1.1.1.1.1	Yes	Yes
Digital Mammography X-Ray Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.2	Yes	Yes
Digital Mammography X-Ray Image Storage – for Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Yes	Yes
Digital Intra-oral X-Ray Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.3	Yes	Yes
Digital Intra-oral X-Ray Image Storage – for Processing	1.2.840.10008.5.1.4.1.1.1.3.1	Yes	Yes
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Yes	Yes
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	Yes	Yes
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Yes	Yes
Multi-frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	Yes	Yes
Multi-frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	Yes	Yes
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	Yes	Yes
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	Yes	Yes
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	Yes	Yes
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	Yes	Yes
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	Yes	Yes
Raw Data Storage	1.2.840.10008.5.1.4.1.1.66	Yes	Yes
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	Yes	Yes
Encapsulated PDF	1.2.840.10008.5.1.4.1.1.104.1	Yes	Yes
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	Yes	Yes
RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1	Yes	Yes
RT Structure Set Storage	1.2.840.10008.5.1.4.1.1.481.3	Yes	Yes
RT Plan Storage	1.2.840.10008.5.1.4.1.1.481.5	Yes	Yes

SOP Class		User of Service (SCU)	Provider of Service (SCP)
Name	UID		
<b>Query/Retrieve</b>			
Study Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	Yes	Yes
Study Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Yes	Yes
<b>Workflow Management</b>			
Storage Commitment Push Model	1.2.840.10008.1.20.1	Yes	No
<b>Print Management</b>			
Basic Film Session	1.2.840.10008.5.1.1.1	Yes	No
Basic Film Box	1.2.840.10008.5.1.1.2	Yes	No
Basic Grayscale Image Box	1.2.840.10008.5.1.1.4	Yes	No
Basic Color Image Box	1.2.840.10008.5.1.1.4.1	Yes	No
Basic Grayscale Print Management (Meta)	1.2.840.10008.5.1.1.9	Yes	No
Printer	1.2.840.10008.5.1.1.16	Yes	No
Basic Color Print Management (Meta)	1.2.840.10008.5.1.1.18	Yes	No

*Note: Verification SCP (C-ECHO) is not included in the table above because it is required for any Acceptor of an Association. The Verification SCU details are covered in the details of the conformance statement.*

**Table 2: Media Services**

Media Storage Application Profile	Write Files (FSC or FSU)	Read Files (FSR)
<b>Compact Disk – Recordable</b>		
CT/MR Studies on CD-R	Yes	Yes
STD-GEN-CD	Yes (FSC only)	Yes

## 2. TABLE OF CONTENTS

1.	<b>DICOM CONFORMANCE STATEMENT OVERVIEW</b>	<b>3</b>
2.	<b>TABLE OF CONTENTS</b>	<b>5</b>
3.	<b>INTRODUCTION</b>	<b>9</b>
3.1.	<b>REVISION HISTORY</b>	<b>9</b>
3.2.	<b>AUDIENCE</b>	<b>9</b>
3.3.	<b>REMARKS</b>	<b>9</b>
3.4.	<b>DEFINITIONS, TERMS AND ABBREVIATIONS</b>	<b>10</b>
3.5.	<b>REFERENCES</b>	<b>11</b>
4.	<b>NETWORKING</b>	<b>12</b>
4.1.	<b>IMPLEMENTATION MODEL</b>	<b>12</b>
4.1.1.	Application Data Flow	12
4.1.2.	Functional Definition of AE's	13
4.1.2.1.	Functional Definition of DICOM Manager	14
4.1.2.2.	Functional Definition of Print Manager	15
4.2.	<b>AE SPECIFICATIONS</b>	<b>16</b>
4.2.1.	DICOM Manager	16
4.2.1.1.	SOP Classes	16
4.2.1.2.	Association Policies	17
4.2.1.2.1.	General	17
4.2.1.2.2.	Number of Associations	17
4.2.1.2.3.	Asynchronous Nature	17
4.2.1.2.4.	Implementation Identifying Information	17
4.2.1.2.5.	Communication Failure Handling	18
4.2.1.3.	Association Initiation Policy	18
4.2.1.3.1.	(Real-World) Activity – Verification (C-ECHO)	20
4.2.1.3.2.	(Real-World) Activity – Storage (C_STORE)	21
4.2.1.3.3.	(Real-World) Activity – Storage Commitment	24
4.2.1.3.4.	(Real-World) Activity – DICOM-Manager C-FIND (SCU)	27
4.2.1.3.5.	(Real-World) Activity – DICOM-Manager C-MOVE (SCU)	30
4.2.1.4.	Association Acceptance Policy	32
4.2.1.4.1.	(Real-World) Activity – DICOM Manager (C-ECHO SCP)	33
4.2.1.4.2.	(Real-World) Activity – DICOM Manager (C-STORE SCP)	34
4.2.1.4.3.	(Real-World) Activity – DICOM Manager (C-FIND SCP)	37
4.2.1.4.4.	(Real-World) Activity – DICOM Manager (C-MOVE SCP)	39
4.2.2.	Print-Manager Specifications	41
4.2.2.1.	SOP Classes	41
4.2.2.2.	Association Policies	41
4.2.2.2.1.	General	41
4.2.2.2.2.	Number of Associations	41
4.2.2.2.3.	Asynchronous Nature	41
4.2.2.2.4.	Implementation Identifying Information	42
4.2.2.3.	Association Initiation Policy	42
4.2.2.3.1.	(Real-World) Activity – Print Manager>	42
4.2.2.4.	Association Acceptance Policy	49
4.3.	<b>NETWORK INTERFACE</b>	<b>49</b>
4.3.1.	Physical Network Interface	49
4.3.2.	Additional Protocols	49

<b>4.4.</b>	<b>CONFIGURATION .....</b>	<b>50</b>
4.4.1.	AE Title/Presentation Address Mapping .....	50
4.4.1.1.	Local AE Titles .....	51
4.4.1.2.	Remote AE Title/Presentation Address Mapping .....	51
4.4.2.	Parameters.....	51
<b>5.</b>	<b>MEDIA INTERCHANGE.....</b>	<b>52</b>
<b>5.1.</b>	<b>IMPLEMENTATION MODEL .....</b>	<b>52</b>
5.1.1.	Application Data Flow Diagram.....	52
5.1.2.	Functional Definitions of AE's .....	52
5.1.3.	Sequencing of Real World Activities .....	52
5.1.4.	File Meta Information for Implementation Class and Version.....	53
<b>5.2.</b>	<b>AE SPECIFICATIONS .....</b>	<b>53</b>
5.2.1.	Media AE - Specification .....	53
5.2.1.1.	File Meta Information for the Media AE .....	53
5.2.1.2.	Real-World Activities .....	53
5.2.1.2.1.	Display Directory.....	53
5.2.1.2.2.	Write Images.....	54
5.2.1.3.	DICOMDIR keys.....	54
5.2.1.3.1.	Read Images.....	56
<b>5.3.</b>	<b>AUGMENTED AND PRIVATE APPLICATION PROFILES .....</b>	<b>56</b>
5.3.1.	Augmented Application Profiles .....	56
5.3.2.	Private Application Profiles .....	56
<b>5.4.</b>	<b>MEDIA CONFIGURATION .....</b>	<b>56</b>
<b>6.</b>	<b>SUPPORT OF CHARACTER SETS .....</b>	<b>57</b>
<b>7.</b>	<b>SECURITY.....</b>	<b>58</b>
<b>7.1.</b>	<b>SECURITY PROFILES .....</b>	<b>58</b>
<b>7.2.</b>	<b>ASSOCIATION LEVEL SECURITY.....</b>	<b>58</b>
<b>7.3.</b>	<b>APPLICATION LEVEL SECURITY .....</b>	<b>58</b>
<b>8.</b>	<b>ANNEXES.....</b>	<b>59</b>
<b>8.1.</b>	<b>CT IOD CONTENTS.....</b>	<b>59</b>
8.1.1.	Created SOP Instances .....	59
8.1.1.1.	General Rules .....	59
8.1.1.2.	SC Image IOD Modules .....	59
8.1.1.3.	Key Object Selection Document IOD Modules .....	60
8.1.1.4.	Encapsulated PDF IOD Modules .....	60
8.1.2.	Attribute Mapping .....	61
8.1.3.	Coerced/Modified fields.....	61
<b>8.2.</b>	<b>PET IOD CONTENTS .....</b>	<b>62</b>
8.2.1.	Created SOP Instances .....	62
8.2.1.1.	General Rules .....	62
8.2.1.2.	PET Image IOD .....	62
8.2.1.3.	NM Image IOD .....	63
8.2.1.4.	Secondary Capture Image IOD.....	63
8.2.1.5.	Multi-Frame Grayscale Byte Secondary Capture Image IOD.....	64
8.2.1.6.	True-Color Secondary Capture Image IOD .....	65
8.2.1.7.	RT Structure Sets IOD .....	65
8.2.1.8.	PET Modules.....	73
8.2.1.9.	NM Modules .....	76
8.2.1.10.	Secondary Capture Modules .....	79
8.2.1.11.	RT Structure Modules.....	80
8.2.2.	Usage of Attributes from Received IODs.....	81
8.2.3.	Attribute Mapping .....	81
8.2.4.	Coerced/Modified Fields .....	81

---

<b>8.3.</b>	<b>DATA DICTIONARIES.....</b>	<b>82</b>
<b>8.4.</b>	<b>CODED TERMINOLOGY AND TEMPLATES.....</b>	<b>83</b>
8.4.1.	GEMINI TF Templates .....	83
8.4.2.	Content Groups.....	83
8.4.3.	PET Coded Terminology.....	83
<b>8.5.</b>	<b>GRAYSCALE IMAGE CONSISTENCY.....</b>	<b>84</b>
<b>8.6.</b>	<b>STANDARD EXTENDED/SPECIALIZED/PRIVATE SOPS.....</b>	<b>84</b>
<b>8.7.</b>	<b>PRIVATE TRANSFER SYNTAXES.....</b>	<b>84</b>





## 3. INTRODUCTION

The introduction specifies product and relevant disclaimers as well as any general information that the vendor feels is appropriate.

### 3.1. Revision History

The revision history provides dates and differences of the different releases.

**Table 3: Revision History**

Document Version	Date of Issue	Author	Description
Rev A	June 15, 2006	PET NM Tech Pubs	GEMINI TF Version 3.0 Initial Release
Rev B	August 18, 2006	PET NM Tech Pubs	GEMINI TF Version 3.1 Release

### 3.2. Audience

This Conformance Statement is intended for:

- (Potential) customers
- System integrators of medical equipment
- Marketing staff interested in system functionality
- Software designers implementing DICOM interfaces

It is assumed that the reader is familiar with the DICOM standard.

### 3.3. Remarks

The DICOM Conformance Statement is contained in chapter 4 through 8 and follows the contents and structuring requirements of [DICOM] PS 3.2.

This DICOM Conformance Statement by itself does not guarantee successful interoperability of Philips equipment with non-Philips equipment. The user (or user's agent) should be aware of the following issues:

- **Interoperability**  
Interoperability refers to the ability of application functions, distributed over two or more systems, to work successfully together. The integration of medical devices into an IT environment may require application functions that are not specified within the scope of DICOM. Consequently, using only the information provided by this Conformance Statement does not guarantee interoperability of Philips equipment with non-Philips equipment.  
It is the user's responsibility to analyze thoroughly the application requirements and to specify a solution that integrates Philips equipment with non-Philips equipment.

- **Validation**

Philips equipment has been carefully tested to assure that the actual implementation of the DICOM interface corresponds with this Conformance Statement.

Where Philips equipment is linked to non-Philips equipment, the first step is to compare the relevant Conformance Statements. If the Conformance Statements indicate that successful information exchange should be possible, additional validation tests will be necessary to ensure the functionality, performance, accuracy and stability of image and image related data. It is the responsibility of the user (or user's agent) to specify the appropriate test suite and to carry out the additional validation tests.

- **New versions of the DICOM Standard**

The DICOM Standard will evolve in future to meet the user's growing requirements and to incorporate new features and technologies. Philips is actively involved in this evolution and plans to adapt its equipment to future versions of the DICOM Standard. In order to do so, Philips reserves the right to make changes to its products or to discontinue its delivery.

The user should ensure that any non-Philips provider linking to Philips equipment also adapts to future versions of the DICOM Standard. If not, the incorporation of DICOM enhancements into Philips equipment may lead to loss of connectivity (in case of networking) and incompatibility (in case of media).

### 3.4. Definitions, Terms and Abbreviations

DICOM definitions, terms and abbreviations are used throughout this Conformance Statement. For a description of these, see [DICOM] PS 3.3 and PS 3.4.

The word Philips in this document refers to Philips Medical Systems.

The following acronyms and abbreviations are used in this document.

AE	Application Entity
ANSI	American National Standard Institute
AP	Application Profile
BOT	Basic Offset Table
CD	Compact Disc
CD-R	CD-Recordable
CD-M	CD-Medical
CR	Computed Radiography
CT	Computed Tomography
DCR	Dynamic Cardio Review
DICOM	Digital Imaging and Communications in Medicine
DIMSE	DICOM Message Service Element
DIMSE-C	DIMSE-Composite
DIMSE-N	DIMSE-Normalized
DVD	Digital Versatile Disc
DX	Digital X-Ray
EBE	DICOM Explicit VR Big Endian
ELE	DICOM Explicit VR Little Endian
FSC	File-set Creator
FSR	File-set Reader
FSU	File-set Updater
GUI	Graphic User Interface

---

HIS	Hospital Information System
HL7	Health Level Seven
ILE	DICOM Implicit VR Little Endian
IOD	Information Object Definition
ISIS	Information System – Imaging System
MOD	Magneto-Optical Disk
MPPS	Modality Performed Procedure Step
MR	Magnetic Resonance
NEMA	National Electrical Manufacturers Association
NM	Nuclear Medicine
PDU	Protocol Data Unit
PET	Positron Emission Tomography
RF	X-Ray Radiofluoroscopic
RIS	Radiology Information System
RT	Radiotherapy
RWA	Real-World Activity
SC	Secondary Capture
SCM	Study Component Management
SCP	Service Class Provider
SCU	Service Class User
SOP	Service Object Pair
TCP/IP	Transmission Control Protocol/Internet Protocol
UID	Unique Identifier
US	Ultrasound
USMF	Ultrasound Multi-frame
WLM	Worklist Management
XA	X-Ray Angiographic

### 3.5. References

- [DICOM] Digital Imaging and Communications in Medicine (DICOM), Part 1 – 18 (NEMA PS 3.1-2004 – PS 3.18-2004), National Electrical Manufacturers Association (NEMA) Publication Sales 1300 N. 17<sup>th</sup> Street, Suite 1847 Rosslyn, Virginia. 22209, United States of America.  
Note that at any point in time the official standard consists of the most recent yearly edition of the base standard (currently 2004) PLUS all the supplements and correction items that have been approved as Final Text

---

## 4. NETWORKING

This section contains the networking related services vs. the media related ones in Media Interchange.

### 4.1. Implementation model

The implementation model consists of three sections:

- The application data flow diagram, specifying the relationship between the Application Entities and the “external world” or Real-World Activities,
- A functional description of each Application Entity, and
- The sequencing constraints among them.

#### 4.1.1. Application Data Flow

The system implements and provides DICOM services using the following Application Entities:

- Dicom-Manager
- Print-Manager

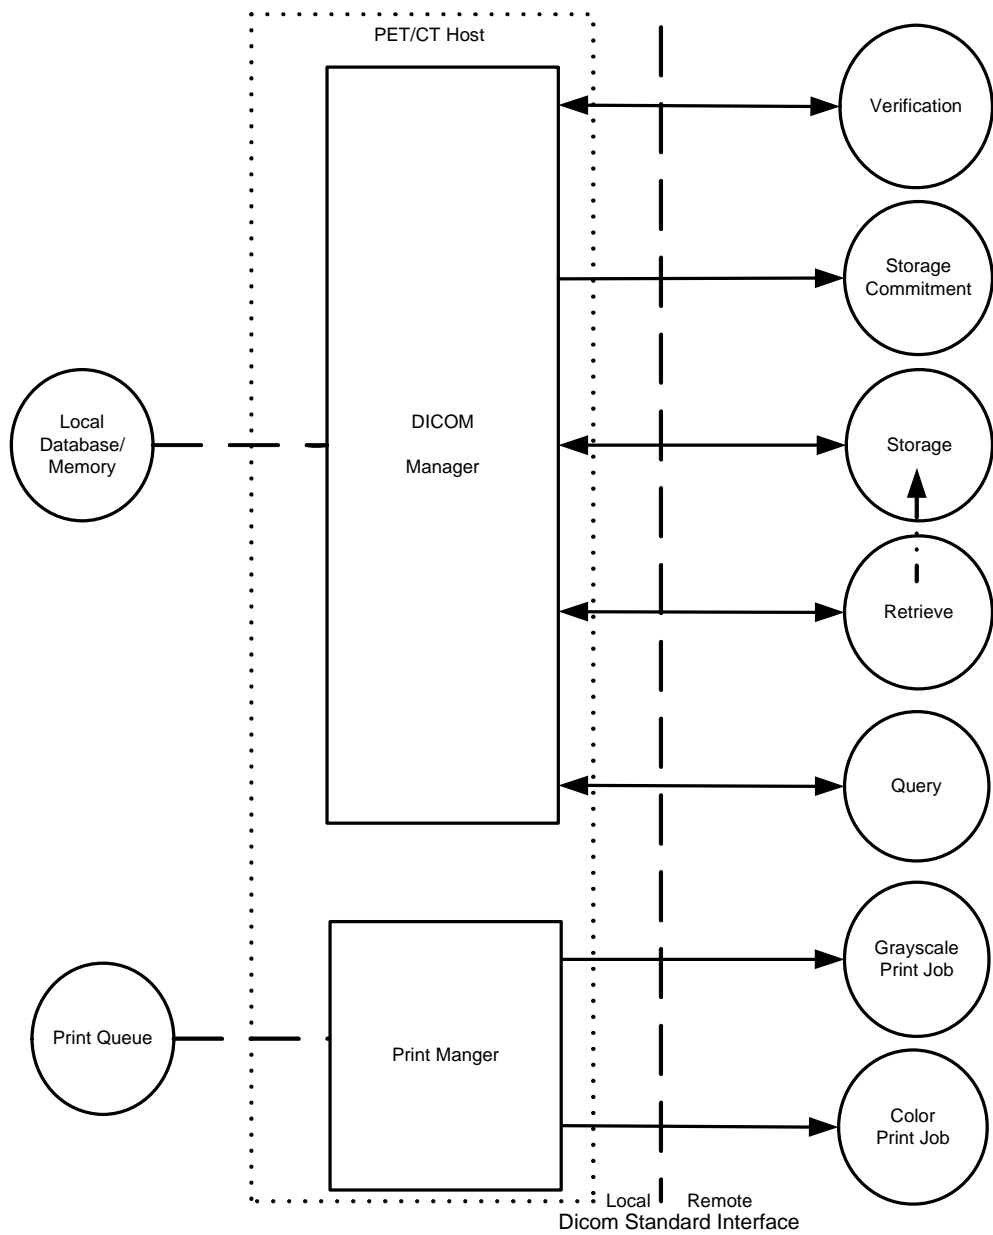


Figure 1: Application Data Flow Diagram

4.1.2. Functional Definition of AE's

This part contains a functional definition for each individual local Application Entity. It describes in general terms the functions to be performed by the AE, and the DICOM services used to accomplish these functions. In this sense, "DICOM services" refers not only to DICOM Service Classes, but also to lower level DICOM services, such as Association Services.

4.1.2.1. Functional Definition of DICOM Manager


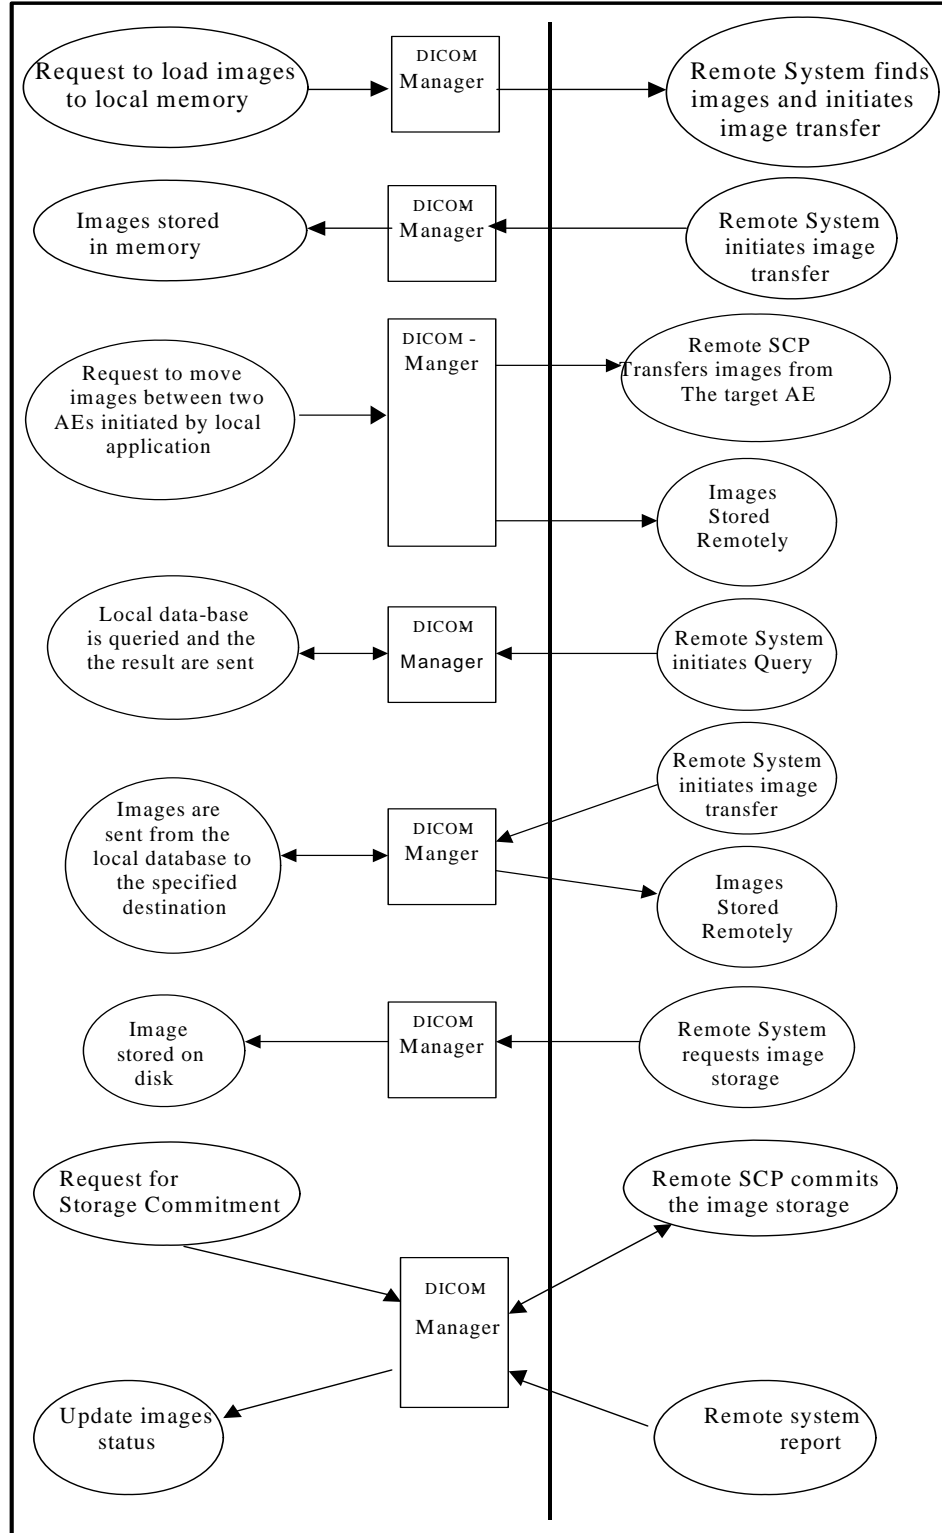


Figure 2: Illustration of DICOM Manager

- The DICOM-Manager is responsible for loading images into memory. The DICOM- Manager gets requests from local image processing and display applications to load images to the memory. It performs these requests using the Query-Retrieve Service Class (C-MOVE only).
- The DICOM-Manager waits for another application to connect at the presentation address configured for its AE title. Memory-Server will accept associations with Presentation Contexts for SOP classes of the Storage and Verification Service Classes. It will receive images on these Presentation Contexts and load them into the system's memory.
- The DICOM Manager is responsible to issue and support the storage commitment service as SCU. When some remote storage device server is configured to support this service, The DICOM Manager establishes association with the specified AE title and sends storage commitment (N-ACTION) request using push the model. After that, it may accept storage commitment (N-EVENT-REPORT) requests on the same association or by establishing another association
- The DICOM Manager waits for another application to connect at the presentation address configured for its AE title. The DICOM Manager will accept associations with Presentation Contexts for Service Object Pair (SOP) classes of the Storage, Query-Retrieve (C-MOVE and C-FIND only) and Verification Service Classes.
- When performing a Storage Service Class (SCP), the DICOM Manager will receive images and store them into the system's local database. The same AE may be used (with a configurable different AE title) to access the local MOD or different local hard disk folders.
- When performing Query-Retrieve Service Class (C-FIND SCP), the DICOM Manager will query its local database according to the request's parameters, and will send the results to the issuer.
- When performing Query-Retrieve Service Class (C-MOVE SCP), the DICOM Manager will issue a C-STORE (SCU) to the target AE for every image found according to the request.

#### 4.1.2.2. Functional Definition of Print Manager

The Print-Manager is a Graphical User Interface (GUI) based application. It enables the user to print predefined images using the DICOM protocol. The user can specify as a printing destination one of several predefined printers. The user can also modify some of the printing parameters such as the film size and format. The following figure provides an illustration of Print-Manager activities:

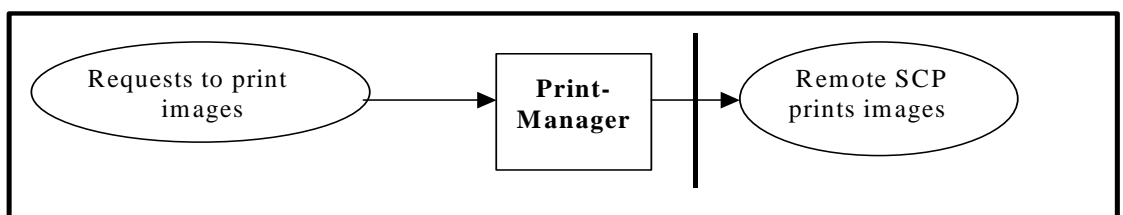

**Figure 3: Illustration of Print Manager**

## 4.2. AE Specifications

The Extended Brilliance Workspace V3.0 consists of two AEs, The DICOM Manager and Print Manager. These two AEs will be described in the subsections 4.2.1 and 4.2.2.

### 4.2.1. DICOM Manager

Every detail of this specific Application Entity shall be completely specified under this section.

#### 4.2.1.1. SOP Classes

This Application Entity provides Standard Conformance to the following SOP Classes.

**Table 4: SOP Classes for DICOM Manager**

SOP Class Name	SOP Class UID	SCU	SCP
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	Yes	Yes
Digital X-Ray Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.1	Yes	Yes
Digital X-Ray Image Storage – for Processing	1.2.840.10008.5.1.4.1.1.1.1.1	Yes	Yes
Digital Mammography X-Ray Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.2	Yes	Yes
Digital Mammography X-Ray Image Storage – for Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Yes	Yes
Digital Intra-oral X-Ray Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.3	Yes	Yes
Digital Intra-oral X-Ray Image Storage – for Processing	1.2.840.10008.5.1.4.1.1.1.3.1	Yes	Yes
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Yes	Yes
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	Yes	Yes
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Yes	Yes
Multi-frame Grayscale Byte Secondary Capture Image Storage (**)	1.2.840.10008.5.1.4.1.1.7.2	Yes	Yes
Multi-frame True Color Secondary Capture Image Storage (**)	1.2.840.10008.5.1.4.1.1.7.4	Yes	Yes
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	Yes	Yes
Grayscale Softcopy Presentation State Storage (*)	1.2.840.10008.5.1.4.1.1.11.1	Yes	Yes
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	Yes	Yes
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	Yes	Yes
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	Yes	Yes
Raw Data Storage (*)	1.2.840.10008.5.1.4.1.1.66	Yes	Yes
Key Object Selection Document (*)	1.2.840.10008.5.1.4.1.1.88.59	Yes	Yes
Encapsulated PDF (*)	1.2.840.10008.5.1.4.1.1.104.1	Yes	Yes
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	Yes	Yes
RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1	Yes	Yes
RT Structure Set Storage	1.2.840.10008.5.1.4.1.1.481.3	Yes	Yes
RT Plan Storage	1.2.840.10008.5.1.4.1.1.481.5	Yes	Yes
Study Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	Yes	Yes



SOP Class Name	SOP Class UID	SCU	SCP
Study Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Yes	Yes
Storage Commitment Push Model	1.2.840.10008.1.20.1	Yes	No
Verification SOP Class	1.2.840.10008.1.1	Yes	Yes

**Notes:**

(\*) These SOP Classes are only supported for storage (not for viewing/processing)

(\*\*) These SOP Classes are supported for storage; they are also supported for viewing/processing by certain optional applications when installed on the system

#### 4.2.1.2. Association Policies

##### 4.2.1.2.1. General

The DICOM standard application context shall be specified.

**Table 5: DICOM Application Context**

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

##### 4.2.1.2.2. Number of Associations

The number of simultaneous associations that will be accepted by DICOM Manager is limited on 50.

**Table 6: Number of Associations as an Association Initiator for DICOM-Manager**

Maximum number of simultaneous associations	Unlimited
---	-----------

**Table 7: Number of Associations as an Association Acceptor for DICOM-Manager**

Maximum number of simultaneous associations	50
---	----

##### 4.2.1.2.3. Asynchronous Nature

If the implementation supports negotiation of multiple outstanding transactions this is stated here, along with the maximum number of outstanding transactions supported.

**Table 8: Asynchronous Nature as an Association Initiator for DICOM-Manager**

Maximum number of outstanding asynchronous transactions	1
---	---

##### 4.2.1.2.4. Implementation Identifying Information

The value supplied for Implementation Class UID is documented here. If a version name is supplied, this fact is documented here. Policies defining the values supplied for version name may be stated here.

**Table 9: DICOM Implementation Class and Version for DICOM-Manager**

Implementation Class UID	1.3.46.670589.33.1.1
Implementation Version Name	BRCONN_3.0

#### 4.2.1.2.5. Communication Failure Handling

The behavior of the AE during communication failure is summarized in Table 10.

**Table 10: Communication Failure Behavior**

Exception	Behavior
ARTIM Timeout	The system stops the ARTIM timer and close the transport connection
Association Timeout	A release request is sent in order to close the association

#### 4.2.1.3. Association Initiation Policy

This describes the conditions under which the AE will initiate an association.

The behavior of the AE during association rejection is summarized in Table 11.

**Table 11: DICOM Association Rejection Handling**

Result	Source	Reason/Diagnosis	Behavior
1 – rejected-permanent	1 – DICOM UL service-user	1 – no-reason-given	The connection is closed
		2 – application-context-name-not-supported	The connection is closed
		3 – calling-AE-title-not-recognized	The connection is closed
		7 – called-AE-title-not-recognized	The connection is closed
	2 – DICOM UL service-provider (ACSE related function)	1 – no-reason-given	The connection is closed
		2 – protocol-version-not-supported	The connection is closed
		3 – DICOM UL service-provider (presentation related function)	1 – temporary-congestion
2 – rejected-transient	1 – DICOM UL service-user	1 – no-reason-given	The connection is closed
		2 – application-context-name-not-supported	The connection is closed
		3 – calling-AE-title-not-recognized	The connection is closed
		7 – called-AE-title-not-recognized	The connection is closed
	2 – DICOM UL service-provider (ACSE related function)	1 – no-reason-given	The connection is closed
		2 – protocol-version-not-supported	The connection is closed
		3 – DICOM UL service-provider (presentation related function)	1 – temporary-congestion
		2 – local-limit-exceeded	The connection is closed

The behavior of the AE on receiving an association abort is summarized in Table 12.

**Table 12: DICOM Association Abort Handling**

Source	Reason/Diagnosis	Behavior
0 – DICOM UL service-user	0 – reason-not-specified	The connection is closed
2 – DICOM UL service-provider	0 – reason-not-specified	The connection is closed
	1 – unrecognized-PDU	The connection is closed
	2 – unexpected-PDU	The connection is closed
	4 – unrecognized-PDU parameter	The connection is closed
	5 – unexpected-PDU parameter	The connection is closed
	6 – invalid-PDU-parameter value	The connection is closed


The behavior of the AE for sending an association abort is summarized in Table 13.

**Table 13: DICOM Association Abort Policies**

Source	Reason/Diagnosis	Behavior
0 – DICOM UL service-user	0 – reason-not-specified	When the system tries to disconnect before receiving an association accept but after sending association request
		When receiving association accept with no presentation context item
		When receiving association accept where all items in the presentation context item list are not accepted by remote system
		When an association timeout (configurable per remote device) expired (timeout which determines how long to keep an idle association).
		When receiving a PDU whose size is bigger than the agreed max PDU size
2 – DICOM UL service-provider	1 – unrecognized-PDU	When ever the system receives unexpected or unrecognized PDU (according to the DICOM UPPER LAYER PROTOCOL STATE TRANSITION TABLE in chapter 8 of the DICOM standard).

**4.2.1.3.1. (Real-World) Activity – Verification (C-ECHO)**

**4.2.1.3.1.1. Description and Sequencing of Activities**

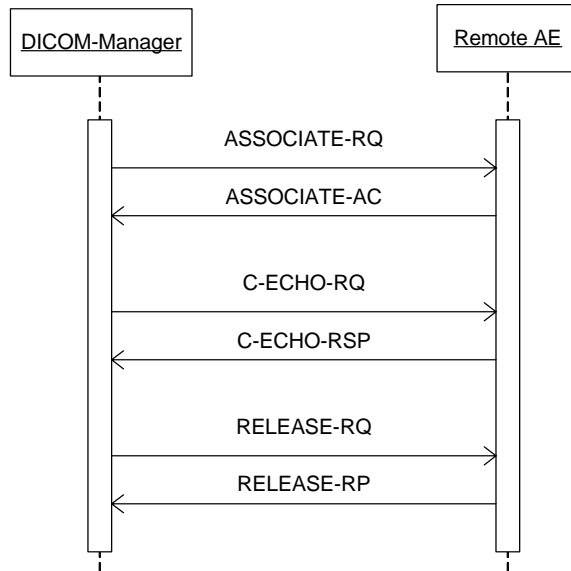

**Figure 4: (Real World) Activity – DICOM Manager (C-ECHO SCU)**

DICOM Manager initiates an association when the user points to one of the icons in the devices tool-bar, clicks the right mouse button and selects “Verify Connection” operation.

**4.2.1.3.1.2. Proposed Presentation Contexts**

Each time an association is initiated, the association initiator proposes a number of presentation contexts to be used on that association. In this subsection, the presentation contexts proposed by DICOM Manager for (Real-World) Activity – Verification (C-ECHO) are defined in Table 14

**Table 14: Proposed Presentation Contexts for (Real-World) Activity – DICOM Manager – C-ECHO SCU**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Verification SOP Class	1.2.840.10008.1.1	ELE	1.2.840.10008.1.2.1	SCU	None
		ILE	1.2.840.10008.1.2		

**4.2.1.3.1.3. SOP Specific Conformance for SOP Classes**

DICOM Manager provides standard conformance to the DICOM V3.0.


Table 15 provides all specific conformance details, including response behavior to all status codes at the application level and regarding communication errors.

**Table 15: DICOM C-ECHO Command Response Status Handling Behavior**

Service Status	Code	Further Meaning	Behavior
Success	0000	Success	The SCU has successfully sent C-ECHO
Other than Success	<>0000	Problems with sending the C-ECHO	The SCU failed to send the C-ECHO; user is notified

**4.2.1.3.2. (Real-World) Activity – Storage (C\_STORE)**

**4.2.1.3.2.1. Description and Sequencing of Activities**

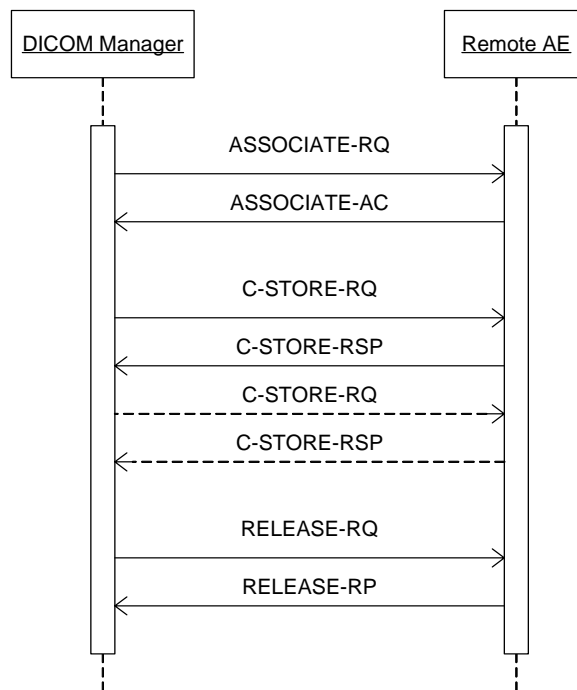

**Figure 5: (Real World) Activity – DICOM Manager (C-STORE SCU)**

The associated Real-World Activity is a request for retrieval of images from the disk/memory and storage of the images to a remote system using a C-STORE command.

**4.2.1.3.2.2. Proposed Presentation Contexts**

Each time an association is initiated, the association initiator proposes a number of presentation contexts to be used on that association. In this subsection, the presentation contexts proposed by DICOM Manager for (Real-World) Activity – DICOM Manager (C-STORE SCU) are defined in Table 16. Explicit VR Transfer Syntaxes for a specific AE target may be restricted using the configuration utility.

**Table 16: Proposed Presentation Contexts for (Real-World) Activity – DICOM Manager – C-STORE SCU**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Digital X-Ray Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Digital X-Ray Image Storage – for Processing	1.2.840.10008.5.1.4.1.1.1.1.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Digital Mammography X-Ray Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.2	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Digital Mammography X-Ray Image Storage – for Processing	1.2.840.10008.5.1.4.1.1.1.2.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Digital Intra-oral X-Ray Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.3	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Digital Intra-oral X-Ray Image Storage – for Processing	1.2.840.10008.5.1.4.1.1.1.3.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Multi-frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Multi-frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Raw Data Storage	1.2.840.10008.5.1.4.1.1.66	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Encapsulated PDF	1.2.840.10008.5.1.4.1.1.104.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
RT Structure Set Storage	1.2.840.10008.5.1.4.1.1.481.3	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
RT Plan Storage	1.2.840.10008.5.1.4.1.1.481.5	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None

DICOM Manager prefers an explicit Transfer Syntax encoding. If offered a choice of Transfer Syntax's in a Presentation Context, it will apply the following priorities to the choice of Transfer Syntax:

- DICOM Explicit VR Little Endian.
- DICOM Implicit VR Little Endian.

#### 4.2.1.3.2.3. SOP Specific Conformance for SOP Classes

DICOM Manager provides standard conformance to the DICOM V3.0 Storage Service Class as an SCU for SOP Classes mentioned in the previous section.

Multiple C-STORE operations can be performed over a single association. Upon receiving a C-STORE confirmation containing a successful status, this implementation will perform the next C-STORE operation (if this operation is the result of the Series Level Move request). The association will be kept open if possible.

Any unsuccessful status (error or warning), returned in the C-STORE confirmation, results in termination of sending further C-Store requests (if any in the queue) and reporting of the error to the system log file.

There are two timeouts for the association. One timeout, "Association Timeout" is used to close an idle association. For C-Store the default is 120 sec but it can be configured per remote node. The other timeout is "Service Timeout" which detects that no data is transmitted over the association and closes it. The default for C-Store is 5 minutes.

The system creates CT, PET, NM, Single and Multi-frame Secondary Capture Images and RT Structure Sets. In sections 8.1.1 and 8.2.1 detailed descriptions of the created objects are defined.

All details regarding the specific conformance, including response behavior to all status codes, both from an application level and communication errors are provided in Table 17.


**Table 17: DICOM C-STORE Command Response Status Handling Behavior**

Service Status	Code	Further Meaning	Behavior
Success	0000	Success	Storage successful.

Service Status	Code	Further Meaning	Behavior
Failure	0122	Refused – SOP Class not supported	Message by transfer result – Unknown reason
	A700	Refused – Out of Resources	Message by transfer result – Out of Resources
	A900	Error - Data Set does not match SOP	Message by transfer result – Unknown reason
	C000	Error – Cannot understand	Message by transfer result – Store failed
Warning	B000	Coercion of Data Elements	Warning status is treated as success
	B006	Elements Discarded	Warning status is treated as success
	B007	Data Set does not match	Warning status is treated as success

**4.2.1.3.3. (Real-World) Activity – Storage Commitment**

**4.2.1.3.3.1. Description and Sequencing of Activities**

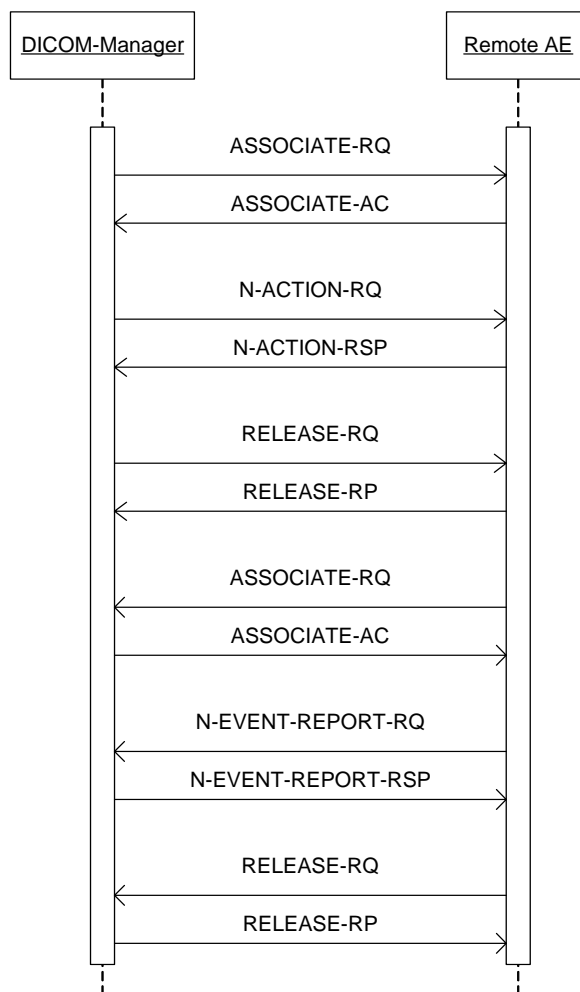

**Figure 6: (Real World) Activity – DICOM Manager (Storage Commitment)**



DICOM-Manager will attempt to initiate a new association when requested to commit the images that were stored on a remote device, which supports the storage Commitment Service.

The associated real world activity for the N-ACTION is a storage commitment request to the remote storage device.

The associated real world activity for the N-EVENT-REPORT operation is the completion of the storage commitment by the remote device. DICOM-Manager will issue a failure status if it is unable to properly handle the storage commitment report event.

**4.2.1.3.3.2. Proposed Presentation Contexts**

Each time an association is initiated, the association initiator proposes a number of presentation contexts to be used on that association. In this subsection, the presentation contexts proposed by DICOM Manager for (Real-World) Activity – Storage Commitment are defined in Table 18

**Table 18: Proposed Presentation Contexts for (Real-World) Activity – DICOM Manager – Storage Commitment**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Storage Commitment Push Model SOP Class	1.2.840.10008.1.20.1	ELE	1.2.840.10008.1.2.1	SCU	None
		ILE	1.2.840.10008.1.2		

**4.2.1.3.3.3. SOP Specific Conformance for SOP Classes**

DICOM-Manager provides standard conformance to the DICOM V3.0 Storage Commitment Service Class using Push Model as an SCU.

Multiple N-ACTION requests can be performed over a single association. Multiple N-EVENT-REPORT requests can be accepted over a single association. After all N-ACTION requests that are waiting in the stack are issued, association will be closed with the timeout of 60 seconds.

A remote system reports about storage commitment completion using N-EVENT-REPORT command. The system can also accept the N-EVENT-REPORT commands over a separate association initiated by the remote system, using reverse role negotiation.

All details regarding the specific conformance, including response behavior to all status codes, both from an application level and communication errors are provided in Table 19 for N-ACTION and in Table 21 for N-EVENT-REPORT

**Table 19: DICOM N-ACTION Command Response Status Handling Behavior**

Service Status	Code	Further Meaning	Behavior
Success	0000	Success	The request for storage commitment is considered successfully stored
Other than Success	<>0000	Problems with sending the N-ACTION	The association is aborted and the request for storage commitment is marked as failed

**Table 20: Storage Commitment N-EVENT-REPORT Behavior**

Event Type Name	Event Type	Behavior
Storage Commitment Request Successful	1	Successfully committed instances are marked as "transferred"
Storage Commitment Request Complete – Failures Exist	2	

**Table 21: DICOM N-EVENT-REPORT Command Response Status Handling Behavior**

Service Status	Code	Further Meaning	Behavior
Success	0000	Success	The storage commitment result has been successfully received.
Failure	0211	Unrecognized Operation	The transaction UID in the N-EVENT-REPORT request is not recognized.
	0213	Resource Limitation	The Transaction UID in the N-EVENT-REPORT request has expired.
	0113	No Such Event Type	An invalid Event Type ID was supplied in the N-EVENT-REPORT.
	0110	Processing Failure	An internal error occurred during processing
	0115	Invalid Argument Value	One of more SOP Instance UIDs with the Referenced SOP Sequence (0008.1199) or Failed SOP Sequence (0008,1198) was not included in the Storage Commitment Request associated with this Transaction UID.

#### 4.2.1.3.4. (Real-World) Activity – DICOM-Manager C-FIND (SCU)

##### 4.2.1.3.4.1. Description and Sequencing of Activities

DICOM-Manager initiates an association when the user clicks on one of the icons in the devices tool-bar.

The DICOM-Manager searches (C-FIND) by Study Level, followed by Series level, and optionally (configurable), by Image Level. The association remains open until the user explicitly closes it by clicking again on the device icon - the Query will be closed with a C-Release

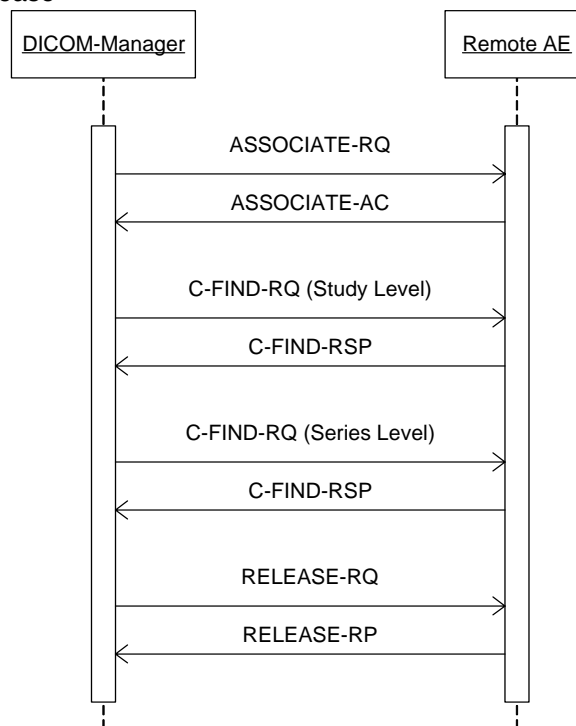


Figure 7: (Real World) Activity – DICOM-Manager C-FIND (SCU)

##### 4.2.1.3.4.2. Proposed Presentation Contexts

Each time an association is initiated, the association initiator proposes a number of presentation contexts to be used on that association. In this subsection, the presentation contexts proposed by Archive-Manager for (Real-World) Activity – DICOM-Manager C-FIND (SCU) are defined in Table 22

**Table 22: Proposed Presentation Contexts for (Real-World) Activity – Archive-Manager C-FIND (SCU)**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Study Root Query /Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None

**4.2.1.3.4.3. SOP Specific Conformance for SOP Classes**

The DICOM-Manager provides standard conformance to the DICOM V3.0. The DICOM-Manager supports the following Study and Series level attributes. Sub-selection on the received list of patients after query will be done on the local memory.

**Table 23: Supported Study and Series Query Level Attributes**

Query Level	Query Key			Value	Type of matching
	Name	Tag	VR		
Study	Specific Character Set	0008,0005	CS	None	None
	Study Date	0008,0020	DA	User Input	S, U, R
	Study Time	0008,0030	TM		None
	Accession Number	0008,0050	SH	User Input	S
	Query/Retrieve Level	0008,0052	CS	STUDY	S
	Modalities in Study	0008,0061	CS	User Input	S
	Referring Physician's Name *	0008,0090	PN	User Input	S, U, *
	Study Description	0008,1030	LO	User Input	S, U, *
	Patient's Name *	0010,0010	PN	User Input	S, U, *
	Patient ID	0010,0020	LO	User Input	S, U, *
	Patient's Birth Date	0010,0030	DA		None
	Patient's Birth Time	0010,0032	TM		None
	Patient's Sex	0010,0040	CS		None
	Study Instance UID	0020,000D	UI		None
	Study ID	0020,0010	SH		None
	Number of Study Related Series	0020,1206	IS		None
	Number of Study Related Images	0020,1208	IS		None
Performed Procedure Step Description	0040,0254	LO		None	
Series	Specific Character Set	0008,0005	CS		None
	Series Date	0008,0021	DA		None
	Series Time	0008,0031	TM		None
	Query/Retrieve Level	0008,0052	CS	SERIES	S
	Modality	0008,0060	CS		None
	Manufacturer	0008,0070	LO		
	Series Description	0008,103E	LO		None

Query Level	Query Key			Value	Type of matching
	Name	Tag	VR		
	Body Part Examined	0018,0015	CS		None
	Protocol Name	0018,1030	LO		None
	Study Instance UID	0020,000D	UI	Parent Study	None
	Series Instance UID	0020,000E	UI		None
	Series Number	0020,0011	IS		None
	Number of Series Related Instances	0020,1209	IS		None
	Performed Procedure Step Start Date	0040,0244	DA		None
	Performed Procedure Step Start Time	0040,0245	TM		None
	Request Attributes Sequence	0040,0275	SQ		None
	>Requested Procedure ID	0040,1001	SH		None
	>Scheduled Procedure Step ID	0040,0009	SH		None
	Image	Specific Character Set	0008,0005	CS	
Image Type		0008,0008	CS		None
Instance Creation Date		0008,0012	DA		None
Instance Creation Time		0008,0013	TM		None
SOP Class UID		0008,0016	UI		None
SOP Instance UID		0008,0018	UI		None
Query/Retrieve Level		0008,0052	CS	IMAGE	S
Contrast Bolus Agent		0018,0010	LO		None
Slice Thickness		0018,0050	DS		None
KVP		0018,0060	DS		None
Series Instance UID		0020,000E	UI		None
Instance Number		0020,0013	IS		None
Patient Orientation		0020,0020	CS		None
Image Orientation Patient		0020,0037	DS		None
Slice Location		0020,1041	DS		None
Sample per Pixel		0028,0002	US		None
Photometric Interpretation		0028,0004	CS		None
Rows		0028,0010	US		None
Columns		0028,0011	US		None
Pixel Spacing		0028,0030	DS		None

\* Note: The column Type of Matching of the table should be read as follows:  
The types of Matching supported by the C-FIND SCP. A "S" indicates the identifier attribute can specify Single Value Matching, a "R" will indicate Range Matching, a "\*" will denote wildcard matching, an "U" will indicate universal matching, and "L" will indicate that UID lists are supported for matching. "NONE" indicates that no matching is supported, but that values for this element in the database can be returned.

All details regarding the specific conformance, including response behavior to all status codes, both from an application level and communication errors are provided in Table 24


**Table 24: DICOM C-FIND Command Response Status Handling Behavior**

Service Status	Code	Further Meaning	Behavior
Success	0000	Success	Matching successful.
Failure	A700	Refused	Out of Resources
	A900	Failed	Unknown reason
	C000	Failed	Unknown reason

**4.2.1.3.5. (Real-World) Activity – DICOM-Manager C-MOVE (SCU)**

**4.2.1.3.5.1. Description and Sequencing of Activities**

DICOM-Manager initiates an association when an image processing application asks for image loading from a specified source device using a proprietary IPC protocol.

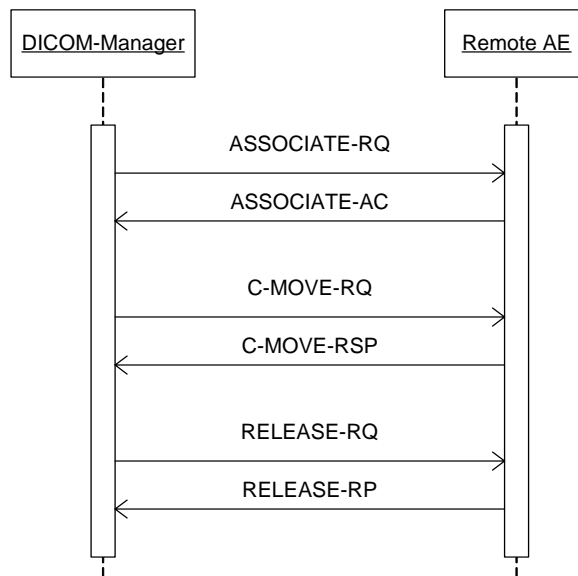

**Figure 8: (Real World) Activity – DICOM-Manager C-MOVE (SCU)**

**4.2.1.3.5.2. Proposed Presentation Contexts**

Each time an association is initiated, the association initiator proposes a number of presentation contexts to be used on that association. In this subsection, the presentation contexts proposed by Memory-Manager for (Real-World) Activity – Memory-Manager C-MOVE (SCU) are defined in Table 25.

**Table 25: Proposed Presentation Contexts for (Real-World) Activity – DICOM-Manager C-MOVE (SCU)**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Study Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	ILE ELE	1.2.840.10008.1.2 1.2.840.10008.1.2.1	SCU	None

**4.2.1.3.5.3. SOP Specific Conformance for SOP Classes**

DICOM-Manager provides standard conformance to the DICOM V3.0 Query/Retrieve Service Class as an SCU for the SOP Class Study Root Query/Retrieve Information Model – Move.

All details regarding the specific conformance, including response behavior to all status codes, both from an application level and communication errors are provided in Table 26.

**Table 26: DICOM C-MOVE Command Response Status Handling Behavior**

Service Status	Code	Further Meaning	Behavior
Success	0000	Success	Storage successful.
Failure	A701	Refused – Out of Resources	Message by transfer result – Refused Unknown reason
	A702	Refused – Out of Resources	Message by transfer result – Refused Store Failed
	A801	Refused – Move Destination Unknown	Message by transfer result – Refused Unknown target
	A900	Error – Identifier Does Not Match SOP Class	Message by transfer result – Failed Unknown reason
	C000	Error – Unable to Process	Message by transfer result – Failed Store Failed
Warning	B000	Sub-operations complete – One or more failures	When ever one of the store operations failed
Cancel	FE00	Cancel	Message by transfer result – Refused Connection closed on timeout.

#### 4.2.1.4. Association Acceptance Policy

Each AE specification shall contain a description of the association acceptance policies of the AE. This describes the conditions under which the AE will accept an association.

The AE association rejection policies are summarized in Table 27.

**Table 27: DICOM Association Rejection Policies**

Result	Source	Reason/Diagnosis	Explanation
1 – rejected-permanent	1 – DICOM UL service-user	2 – application-context-name-not-supported	When receiving association request and the application context name is not supported
		3 – calling-AE-title-not-recognized	When receiving association request and the calling AE title is not supported
		7 – called-AE-title-not-recognized	When receiving association request and the called AE title is not supported
	2 – DICOM UL service-provider (ACSE related function)	1 – no-reason-given	When receiving association request and all of the items in the presentation context item list are not supported by the system
		2 – protocol-version-not-supported	When receiving an association request and the protocol version received is not supported

The behavior of the AE on receiving an association abort is summarized in Table 28.

**Table 28: DICOM Association Abort Policies**


Source	Reason/Diagnosis	Behavior
0 – DICOM UL service-user	0 – reason-not-specified	When the system tries to disconnect before receiving an association accept but after sending association request
		When receiving association accept with no presentation context item
2 – DICOM UL service-provider	1 – unrecognized-PDU	When receiving association accept where all items in the presentation context item list are not accepted by remote system
		When an association timeout (configurable per remote device) expired (timeout which determines how long to keep an idle association).
		When receiving a PDU whose size is bigger than the agreed max PDU size
		When ever the system receives unexpected or unrecognized PDU (according to the DICOM UPPER LAYER PROTOCOL STATE TRANSITION TABLE in chapter 8 of the DICOM standard).



**4.2.1.4.1. (Real-World) Activity – DICOM Manager (C-ECHO SCP)**

**4.2.1.4.1.1. Description and Sequencing of Activities**

A remote system requests verification from DICOM Manager using the C-ECHO command.

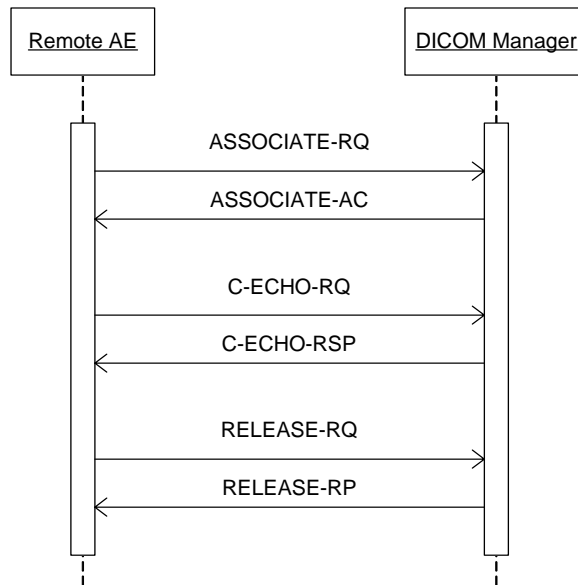

**Figure 9: (Real World) Activity – DICOM Manager (C-ECHO SCP)**

**4.2.1.4.1.2. Accepted Presentation Contexts**

Any of the presentation contexts shown in Table 29 is acceptable to DICOM Manager (C-ECHO SCP).

**Table 29: Acceptable Presentation Contexts for <(Real-World) Activity – DICOM Manager (C-ECHO SCP)**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Verification SOP Class	1.2.840.10008.1.1	ILE ELE	1.2.840.10008.1.2 1.2.840.10008.1.2.1	SCU	None

**4.2.1.4.1.3. SOP Specific Conformance for SOP Classes**

DICOM Manager (C-ECHO SCP) provides standard conformance to the DICOM V3.0 verification SOP Class.


The behavior of an Application Entity SOP class is summarized as shown in Table 30. The standard as well as the manufacturer specific status codes and their corresponding behavior shall be specified.

**Table 30: DICOM Manager (C-ECHO SCP) Status Response**

Service Status	Code	Further Meaning	Description
Success	0000	Success	C-ECHO command was successful received
Other than Success	<>0000	Problems with receiving the C-ECHO	Problems with receiving the C-ECHO

**4.2.1.4.2. (Real-World) Activity – DICOM Manager (C-STORE SCP)**

**4.2.1.4.2.1. Description and Sequencing of Activities**

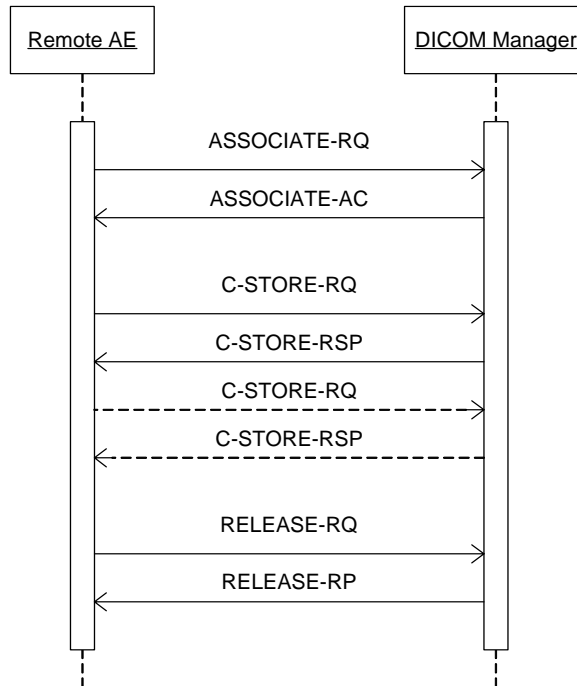

**Figure 10: (Real World) Activity – DICOM Manager C-STORE (SCP)**

The real world activity associated with the C-STORE operation is the storage of the image in the memory of the system upon which DICOM Manager is running in order to make it available for immediate processing by applications. DICOM Manager will issue a failure status if it is unable to store the image in the memory.

#### 4.2.1.4.2.2. Accepted Presentation Contexts

Any of the Presentation Contexts shown in Table 31 is acceptable to the DICOM Manager C-STORE as SCP.

**Table 31: Acceptable Presentation Contexts for (Real-World) Activity – DICOM Manager (C-STORE SCP)**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
Digital X-Ray Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
Digital X-Ray Image Storage – for Processing	1.2.840.10008.5.1.4.1.1.1.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
Digital Mammography X-Ray Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.2	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
Digital Mammography X-Ray Image Storage – for Processing	1.2.840.10008.5.1.4.1.1.1.2.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
Digital Intra-oral X-Ray Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.3	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
Digital Intra-oral X-Ray Image Storage – for Processing	1.2.840.10008.5.1.4.1.1.1.3.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
Multi-frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
Multi-frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
Raw Data Storage	1.2.840.10008.5.1.4.1.1.66	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
Encapsulated PDF	1.2.840.10008.5.1.4.1.1.104.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None
RT Structure Set Storage	1.2.840.10008.5.1.4.1.1.481.3	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
RT Plan Storage	1.2.840.10008.5.1.4.1.1.481.5	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCP	None

#### 4.2.1.4.2.3. SOP Specific Conformance for SOP Classes

DICOM Manager provides standard conformance to the DICOM V3.0 Storage Service Class as a SCP.

DICOM Manager conforms to the SOPs of the Storage Service Class at Level 2 (Full). In case of a successful C-STORE, the stored image may be accessed by the processing applications

The user determines the duration of the storage.


If the DICOM Manager returns one of the following status codes, it means that the C-Store has been unsuccessful.

**Table 32: Memory-Server C-STORE (SCP) Status Response**

Service Status	Code	Further Meaning	Description
Success	0000	Successful	When ever the store operation succeeded
Failure	C000	Failed	When ever the store operation failed

**4.2.1.4.3. (Real-World) Activity – DICOM Manager (C-FIND SCP)**

**4.2.1.4.3.1. Description and Sequencing of Activities**

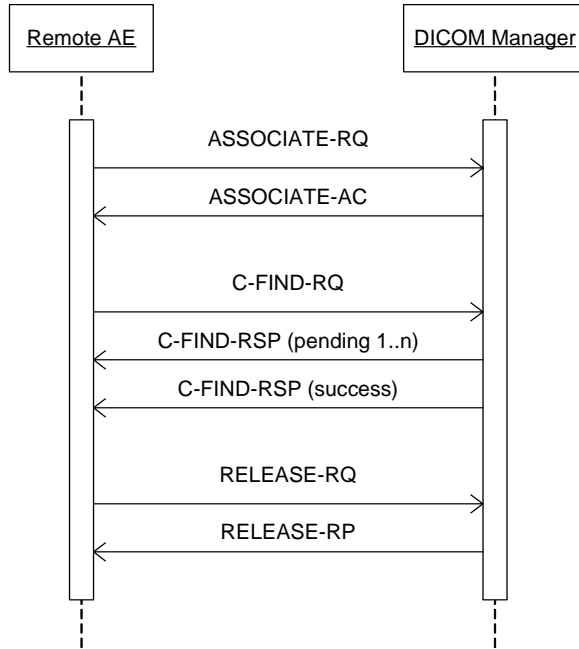

**Figure 11: (Real World) Activity – Disk-Server (C-FIND SCP)**

The Real World activity associated with the C-FIND command is an examination of the disk content. DICOM Manager will issue a failure status if it is unable to process the query request.

**4.2.1.4.3.2. Proposed Presentation Contexts**

Any of the Presentation Contexts show in Table 33 is acceptable to the DICOM Manager (C-FIND SCP).

**Table 33: Proposed Presentation Contexts for <(Real-World) Activity – DICOM Manager (C-FIND SCP)**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	ILE ELE	1.2.840.10008.1.2 1.2.840.10008.1.2.1	SCP	None

#### 4.2.1.4.3.3. SOP Specific Conformance for SOP Classes

DICOM Manager provides standard conformance to the DICOM V3.0 Query/Retrieve Service Class as an SCP for the following SOP Class: Study Root Query/Retrieve Information Model - FIND, UID=1.2.840.10008.5.1.4.1.2.2.1.

Disk-Server does not support Relational Search.

All Required (R) and Unique (U) Study, Series and Image level keys for the Study Root Query/Retrieve Information Model are supported.

Unsupported fields will not be returned in the C-FIND response.

C-FIND-CANCEL is supported. However, some C-FIND responses may be forwarded before the C-FIND-CANCEL takes effect.


All details regarding the specific conformance, including response behavior to all status codes, both from an application level and communication errors are provided in Table 34.

**Table 34: DICOM C-Find Command Response Status Handling Behavior**

Service Status	Code	Further Meaning	Behavior
Success	0000	Matching complete	Matching successful
Failure	C000	General failure status	When ever the find operation failed

**4.2.1.4.4. (Real-World) Activity – DICOM Manager (C-MOVE SCP)**

**4.2.1.4.4.1. Description and Sequencing of Activities**

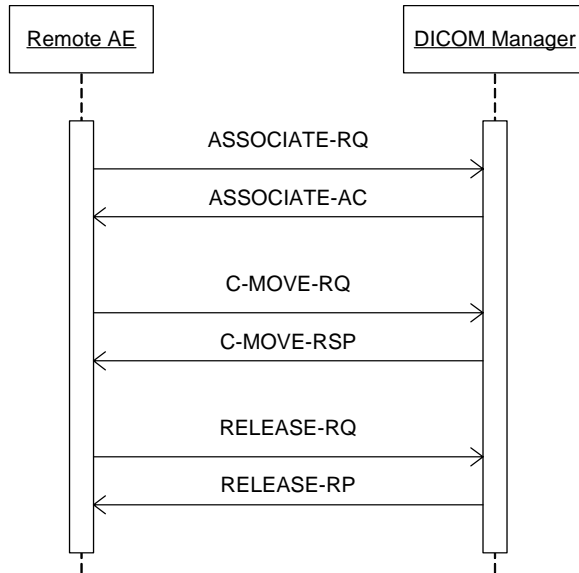

**Figure 12: (Real World) Activity – DICOM Manager (C-MOVE SCP)**

The Real World activity associated with the C-MOVE command is retrieval of images from the disk and storage of the images to a remote system using a C-STORE command. DICOM Manager will issue a failure status if it is unable to process the transfer request

**4.2.1.4.4.2. Proposed Presentation Contexts**

Any of the Presentation Contexts show in Table 35 is acceptable to the DICOM Manager (C-MOVE SCP).

**Table 35: Proposed Presentation Contexts for <(Real-World) Activity – DICOM Manager (C-MOVE SCP)**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Study Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	ILE ELE	1.2.840.10008.1.2 1.2.840.10008.1.2.1	SCP	None

#### 4.2.1.4.4.3. SOP Specific Conformance for SOP Classes

DICOM Manager provides standard conformance to the DICOM V3.0 Query/Retrieve Service Class as an SCP for the following SOP Class: Study Root Query/Retrieve Information Model - MOVE, UID=1.2.840.10008.5.1.4.1.2.2.2.  
Prioritization of C-MOVE requests is not supported.

DICOM Manager does not support relational C-MOVE requests.  
All images requested in the C-MOVE will be sent over a single association (the association will not be established and torn down for each image).

All details regarding the specific conformance, including response behavior to all status codes, both from an application level and communication errors are provided in Table 36

**Table 36: DICOM C-MOVE Command Response Status Handling Behavior**

Service Status	Code	Further Meaning	Behavior
Success	0000	Matching complete	When ever the move operation succeeded.
Failure	A801	Refused – Move Destination Unknown	When ever the move destination is unknown to the system.
	C000	Error – Unable to Process	When ever the move operation failed.
Warning	B000	Sub-operations Complete – One or more Failures	When ever one of the store operations failed.
Pending	FF00	Pending	For every store response received.
Cancel	FE00	Cancel	When receiving a cancel move request.



## 4.2.2. Print-Manager Specifications

### 4.2.2.1. SOP Classes

This Application Entity provides Standard Conformance to the following SOP Classes.

**Table 37: SOP Classes for Print-Manager**

SOP Class Name	SOP Class UID	SCU	SCP
Basic Grayscale Print Management (Meta)	1.2.840.10008.5.1.1.9	Yes	No
>Basic Film Box SOP Class	1.2.840.10008.5.1.1.2	Yes	No
>Basic Film Session SOP Class	1.2.840.10008.5.1.1.1	Yes	No
>Basic Grayscale Image Box SOP Class	1.2.840.10008.5.1.1.4	Yes	No
>Printer SOP Class	1.2.840.10008.5.1.1.16	No	No
Basic Color Print Management (Meta)	1.2.840.10008.5.1.1.18	Yes	No
>Basic Film Box SOP Class	1.2.840.10008.5.1.1.2	Yes	No
>Basic Film Session SOP Class	1.2.840.10008.5.1.1.1	Yes	No
>Basic Color Image Box SOP Class	1.2.840.10008.5.1.1.4.1	Yes	No
>Printer SOP Class	1.2.840.10008.5.1.1.16	No	No

### 4.2.2.2. Association Policies

#### 4.2.2.2.1. General

The maximum PDU Size that the Print-Manager will use is configurable, with a minimum of 2 Kbytes.

**Table 38: DICOM Application Context**

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

#### 4.2.2.2.2. Number of Associations

Print-Manager can have only one open connection at a given time.

**Table 39: Number of Associations as an Association Initiator for Print-Manager**

Maximum number of simultaneous associations	1
---	---

**Table 40: Number of Associations as an Association Acceptor for Print-Manager**

Maximum number of simultaneous associations	0
---	---

#### 4.2.2.2.3. Asynchronous Nature

Print-Manager will only allow a single outstanding operation on an association.

**Table 41: Asynchronous Nature as an Association Initiator for Print-Manager**

Maximum number of outstanding asynchronous transactions	1
---	---

**4.2.2.2.4. Implementation Identifying Information**

The value supplied for Implementation Class UID and Version Name is documented here.

**Table 42: DICOM Implementation Class and Version for Print-Manager**


Implementation Class UID	1.3.46.670589.33.1.1
Implementation Version Name	BRCONN_3.0

**4.2.2.3. Association Initiation Policy**

**4.2.2.3.1. (Real-World) Activity – Print Manager>**

**4.2.2.3.1.1. Description and Sequencing of Activities**

Print-Manager initiates an association when a print job is submitted to a DICOM printer (when the user click on the print button in the film view). The association is left open after the job is completed for a configurable time-out (so that if there are other jobs to the same printer, they will be done on the same association. Jobs to different printers are performed simultaneously.

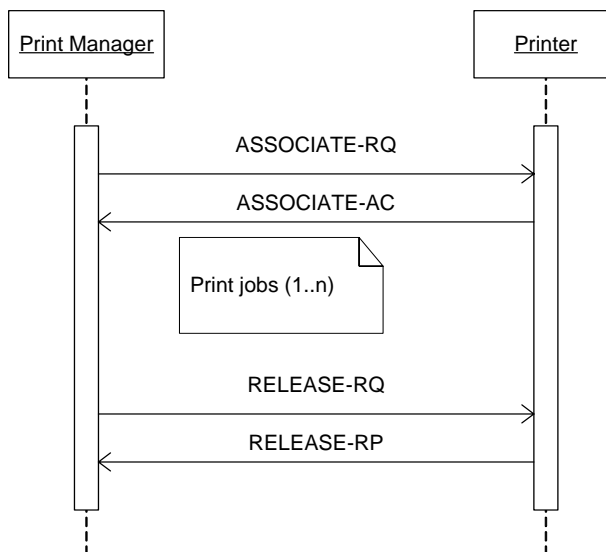

**Figure 13: (Real World) Activity – Print-Manager Initiates**

Normally, when the job is completed and there are no other jobs to the same printer, the print manager does close the association with an A-RELEASE request. If a TCP/IP connection timeout occurs, then the association is closed. In this case, a new association is set up when needed.

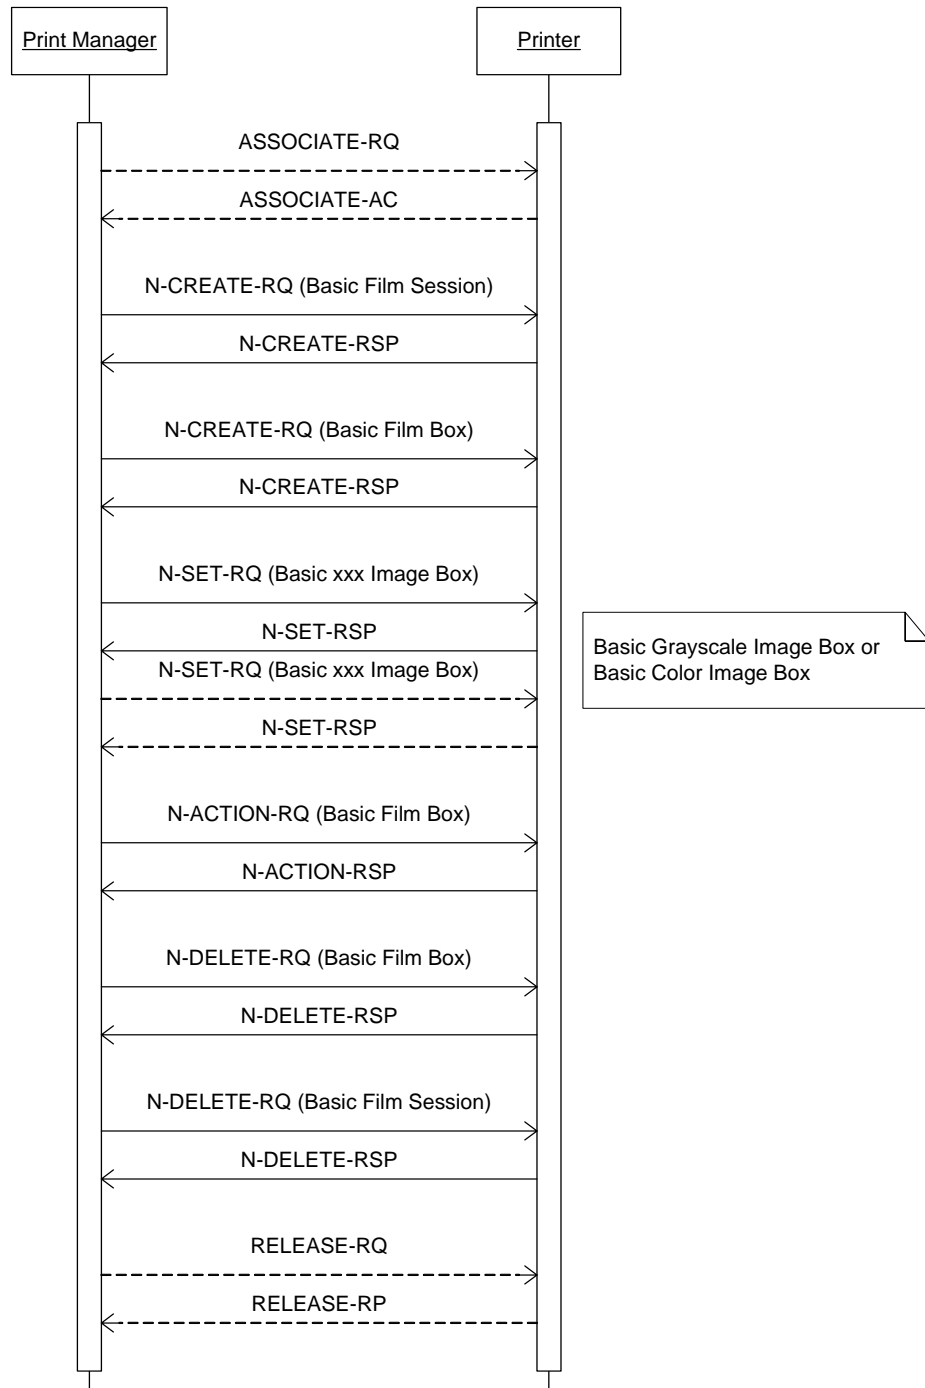


Figure 14: (Real World) Activity – Print-Manager

#### 4.2.2.3.1.2. Proposed Presentation Contexts

Each time an association is initiated, the association initiator proposes a number of presentation contexts to be used on that association. In this subsection, the presentation contexts proposed by Print-Manager for (Real-World) Activity – Print Image are defined in Table 43

**Table 43: Proposed Presentation Contexts for (Real-World) Activity – Print Image**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Basic Grayscale Print Management (Meta)	1.2.840.10008.5.1.1.9	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Basic Color Print Management (Meta)	1.2.840.10008.5.1.1.18	ELE ILE	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None

Recommended abbreviations to be used for the module tables are:

ALWAYS            the attribute is always present with a value  
ANAP                the Attribute is Not Always Present

Recommended abbreviations to be used for the source of the data values in the tables are:

AUTO                the attribute value is generated automatically  
CONFIG              the attribute value source is a configurable parameter

#### 4.2.2.3.1.3. SOP Specific Conformance Basic Film Session SOP Class

The Printer process conforms to the Basic Film Session Sop Class.

The following DIMSE service element is supported:

N-CREATE  
N-DELETE

The following table lists the supported attributes for the N-CREATE DIMSE.

**Table 44: Basic Film Session Presentation Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Number of Copies	2000,0010	IS	1..20	ALWAYS	CONFIG
Print Priority	2000,0020	CS	Printer configuration	ANAP	CONFIG
Medium Type	2000,0030	CS	Printer configuration	ALWAYS	CONFIG
Film Destination	2000,0040	CS	Printer configuration	ALWAYS	CONFIG

The behavior on successful and unsuccessful transfer is given in the table below.

**Table 45: DICOM Command Response Status Handling Behavior for Basic Film Session N-CREATE**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Film Session successfully created	The print job continues
*	B600	Memory Allocation not supported	The print job continues and the warning is logged

**Table 46: DICOM Command Response Status Handling Behavior for Basic Film Session N-DELETE**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Film Session successfully created	The SCP has completed the operation successfully
*		<> 0000	On any other status then success, the job remains in the queue manager, with status failed

#### 4.2.2.3.1.4. SOP Specific Conformance Basic Film Box SOP Class

The Printer process conforms to the Basic Film Box Sop Class.

The following DIMSE service elements are supported:

N-CREATE  
N-ACTION  
N-DELETE

The following table lists the supported attributes for the N-CREATE DIMSE

**Table 47: Basic Film Box Presentation Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Image Display Format	2010,0010	ST	Printer configuration	ALWAYS	CONFIG
Film Orientation	2010,0040	CS	PORTRAIT; LANDSCAPE	ALWAYS	CONFIG
Film Size ID	2010,0050	CS	Printer configuration	ALWAYS	CONFIG
Configuration Information	2010,0150	ST	Printer configuration	ANAP	CONFIG
Trim	2010,0140	CS	NO	ALWAYS	CONFIG

**Table 48: Basic Film Box Relationship Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Referenced Film Session Sequence	2010,0500	SQ		ALWAYS	AUTO
>Referenced SOP Class UID	0008,1150	UI	UID of Parent Film Session	ALWAYS	AUTO
>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	AUTO

The behavior on successful and unsuccessful transfer is given in the table below.

**Table 49: DICOM Command Response Status Handling Behavior for Basic Film Box N-CREATE**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Film Box successfully created	The SCP has completed the operation successfully.
Warning	B605	Requested Min Density or Max Density outside of Printer's operating Range	The print job continues and the warning is logged.
Failure	C616	There is an existing Film Box that has not been printed	The print job is marked as failed and the reason is logged.

N-ACTION DIMSE does not create any Data Set Attributes.

The behavior on successful and unsuccessful transfer is given in the table below.

**Table 50: DICOM Command Response Status Handling Behavior for Basic Film Box N-ACTION**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Film accepted for printing	The print job continues.
Warning	B603	Film Box SOP Instance Hierarchy does not contain Image Box SOP Instances	The print job continues and the warning is logged and reported to the user.
	B604	Image Size is larger than Image Box Size – The Image has been de-magnified	The print job continues and the warning is logged and reported to the user.
	B609	Image Size is larger than Image Box Size – The Image has been cropped to fit	The print job continues and the warning is logged and reported to the user.
	B60A	Image Size or combined Print Image Size is larger than Image Box Size – The Image or combined Print Image has been decimated to fit	The print job continues and the warning is logged and reported to the user.
Failure	C602	Unable to create Print Job SOP Instance – Print Queue is full	The print job is marked as failed and the reason is logged and reported to the user.
	C603	Image Size is larger than Image Box Size	The print job is marked as failed and the reason is logged and reported to the user.
	C613	Combined Print Image Size is larger than Image Box Size	The print job is marked as failed and the reason is logged and reported to the user.

N-DELETE DIMSE does not create any Data Set Attributes.

The behavior on successful and unsuccessful transfer is given in the table below.

**Table 51: DICOM Command Response Status Handling Behavior for Basic Film Box N-DELETE**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Film Session successfully created	The SCP has completed the operation successfully
*		<> 0000	On any other status then success, the job remains in the queue manager, with status failed

#### 4.2.2.3.1.5. SOP Specific Conformance Basic Grayscale Image Box SOP Class

The Printer process conforms to the Basic Grayscale Image Box Sop Class.  
The following DIMSE service element is supported:

N-SET

The following table lists the supported attributes for the N-SET DIMSE

**Table 52: Basic Grayscale Image Box SOP Class - N-SET-RQ - Pixel Presentation Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Image Position	2020,0010	US	1	ALWAYS	AUTO
Basic Grayscale Image Sequence	2020,0110	SQ		ALWAYS	AUTO
>Samples per Pixel	0028,0002	US	1/3	ALWAYS	AUTO
>Photometric Interpretation	0028,0004	CS	MONOCHROME2/ RGB	ALWAYS	AUTO
>Rows	0028,0010	US		ALWAYS	AUTO
>Columns	0028,0011	US		ALWAYS	AUTO
>Pixel Aspect Ratio	0028,0034	IS		ALWAYS	AUTO
>Bits Allocated	0028,0100	US	8, 16	ALWAYS	AUTO
>Bits Stored	0028,0101	US		ALWAYS	AUTO
>High Bit	0028,0102	US		ALWAYS	AUTO
>Pixel Representation	0028,0103	US	0	ALWAYS	AUTO
>Pixel Data	7FE0,0010	OB/OW		ALWAYS	AUTO

The behavior on successful and unsuccessful transfer is given in the table below.

**Table 53: DICOM Command Response Status Handling Behavior for Basic Grayscale Image Box N-SET**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Image successfully stored in Image Box	The print job continues.
Warning	B604	Image Size is larger than Image Box Size – The Image has been de-magnified	The print job continues and the warning is logged and reported to the user.
	B605	Requested Min Density or Max Density outside of Printer's operating Range	The print job continues and the warning is logged and reported to the user.
	B609	Image Size is larger than Image Box Size – The Image has been cropped to fit	The print job continues and the warning is logged and reported to the user.
	B60A	Image Size or combined Print Image Size is larger than Image Box Size – The Image or combined Print Image has been decimated to fit	The print job continues and the warning is logged and reported to the user.
Error	C603	Image Size is larger than Image Box Size	The print job is marked as failed and the reason is logged and reported to the user
	C605	Insufficient Memory in Printer to store the Image	The print job is marked as failed and the reason is logged and reported to the user
	C613	Combined Print Image Size is larger than Image Box Size	The print job is marked as failed and the reason is logged and reported to the user

#### 4.2.2.3.1.6. SOP Specific Conformance Basic Color Image Box SOP Class

The Printer process conforms to the Basic Grayscale Image Box Sop Class.

The following DIMSE service element is:

N-SET

The following table lists the supported attributes for the N-SET DIMSE

**Table 54: Basic Color Image Box SOP Class - N-SET-RQ - Pixel Presentation Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Image Position	2020,0010	US	1	ALWAYS	AUTO
Polarity	2020,0020	CS	Printer configuration	ALWAYS	AUTO
Basic Color Image Sequence	2020,0111	SQ		ALWAYS	AUTO
>Samples per Pixel	0028,0002	US	3	ALWAYS	AUTO
>Photometric Interpretation	0028,0004	CS	RGB	ALWAYS	AUTO
>Planar Configuration	0028,0006	US	0,1	ALWAYS	AUTO
>Rows	0028,0010	US		ALWAYS	AUTO
>Columns	0028,0011	US		ALWAYS	AUTO
>Pixel Aspect Ratio	0028,0034	IS		ALWAYS	AUTO
>Bits Allocated	0028,0100	US	8	ALWAYS	AUTO
>Bits Stored	0028,0101	US	8	ALWAYS	AUTO
>High Bit	0028,0102	US	7	ALWAYS	AUTO
>Pixel Representation	0028,0103	US	0	ALWAYS	AUTO
>Pixel Data	7FE0,0010	OW		ALWAYS	AUTO

The behavior on successful and unsuccessful transfer is given in the Table 55



**Table 55: DICOM Command Response Status Handling Behavior for Basic Color Image Box N-SET**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Image successfully stored in Image Box	The print job continues.
Warning	B604	Image Size is larger than Image Box Size – The Image has been de-magnified	The print job continues and the warning is logged and reported to the user.
	B605	Requested Min Density or Max Density outside of Printer's operating Range	The print job continues and the warning is logged and reported to the user.
	B609	Image Size is larger than Image Box Size – The Image has been cropped to fit	The print job continues and the warning is logged and reported to the user.
	B60A	Image Size or combined Print Image Size is larger than Image Box Size – The Image or combined Print Image has been decimated to fit	The print job continues and the warning is logged and reported to the user.
Error	C603	Image Size is larger than Image Box Size	The print job is marked as failed and the reason is logged and reported to the user.
	C605	Insufficient Memory in Printer to store the Image	The print job is marked as failed and the reason is logged and reported to the user.
	C613	Combined Print Image Size is larger than Image Box Size	The print job is marked as failed and the reason is logged and reported to the user.

#### 4.2.2.4. Association Acceptance Policy

Print-Manager never accepts an association.

### 4.3. Network Interface

#### 4.3.1. Physical Network Interface

The Workspace application provides DICOM V3.0 TCP/IP Network Communication Support as defined in Part 8 of [DICOM].

Extended Brilliance Workspace inherits its TCP/IP stack from Windows XP (i.e. the operating system platform).

Extended Brilliance Workspace supports a single network interface: Ethernet ISO.8802-3.

With standard supported physical medium include:

- IEEE 802.3 10BASE-TX
- IEEE 802.3 100BASE-TX (Fast Ethernet)
- IEEE 802.3 1000BASE-X (Fiber Optic Gigabit Ethernet).

#### 4.3.2. Additional Protocols

Additional protocols such as used for network management are listed here.

## 4.4. Configuration

The Extended Brilliance Workspace system is configured by means of a configuration program. This program is accessible at start-up of the Extended Brilliance Workspace system. It is password protected and intended to be used by the administrator onsite or Philips Customer Support Engineers only.

### 4.4.1. AE Title/Presentation Address Mapping

This mapping (including IP and port numbers) is defined during the system Networking Procedure.

Configurable are the parameters:

- Calling AE Titles
- Called AE Titles
- Maximum PDU size
- Manufacturer
- Model
- Version
- Association timeout
- ARTIM timer
- Large Archive – Force Filter when querying this device
- Archived – Mark studies as Archived when copying them to this device
- Supported Move/Query levels
- Disable explicit transfer syntaxes to be proposed at the association negotiation
- Enable generation of DICOM overlays (“burn-in” instead)

#### 4.4.1.1. Local AE Titles

The local AE title mapping and configuration shall be specified. The default AE titles are based on the system host name defined by the service engineer as part of the system configuration. The following table shall be used:

**Table 56: AE Title Configuration Table**

Application Entity	Default AE Title	Default TCP/IP Port
DICOM-Manager	<hostname> <hostname><localfolder>	104
Print-Manager	<hostname>	

#### 4.4.1.2. Remote AE Title/Presentation Address Mapping

Remote AE Title, IP-Address and Port-number are freely configurable.

#### 4.4.2. Parameters

The specification of important operational parameters, their default value and range (if configurable) is specified here.

**Table 57: Configuration Parameters table**

Parameter	Configurable	Default Value
<b>General Parameters</b>		
Release Timeout	Yes	30 seconds
Port-Number	Yes	104
Maximum PDU size the AE can receive	Yes	16352
Maximum PDU size the AE can send	Yes	16352
Transfer Syntax support, ILE, ELE There is a configuration option to turn off Explicit VR support	Yes	ILE, ELE
Storage / Retrieve Timeout	Yes	5 Minutes
Artim timeout	Yes	5 Minutes
Max association number	Yes	50


Printers are configurable by a selection of the default printer types. Every printer type has a fixed configuration, but it can be extended with new ones. The default printer settings are defined in the printer configuration file.

## 5. MEDIA INTERCHANGE

### 5.1. Implementation Model

AE Provides Standard Conformance to the DICOM Media Storage Service and File Format (PS 3.10) and the Media Storage Application Profiles (PS 3.11)

#### 5.1.1. Application Data Flow Diagram

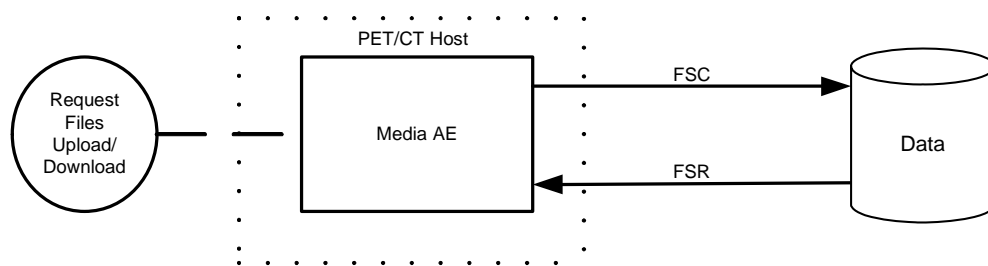

**Figure 15: Media Interchange Application Data Flow Diagram**

The Media AE will act as a FSR when reading the directory of the medium.  
The Media AE will act as a FSC when writing the selected images in a patient folder onto the CD-R medium.

#### 5.1.2. Functional Definitions of AE's

The Media AE includes the following service class.

##### Media Storage Service Class

The Media AE can perform the Media Storage service as SCU, with capabilities for RWA Display Directory (as FSR), RWA Write Images (as FSC), and RWA Read Images (as FSR). The Extended Brilliance Workspace can create and read CD-R and read CD.

#### 5.1.3. Sequencing of Real World Activities

A Real World Activity of the Media AE is:

The user selects a set of object to write these to the CD. Then the CD will be created with the selected objects. Once the CD has been created, the user can read this CD on the Extended Brilliance Workspace or for transport to another device for reading.

Another Real World Activity of the Media AE is:

A CD from another system or previously created can be read by the Extended Brilliance Workspace, but the Extended Brilliance Workspace cannot append to this created CD.

#### 5.1.4. File Meta Information for Implementation Class and Version

**Table 58: DICOM Implementation Class and Version for Media AE**

Implementation Class UID	1.2.46.670589.33.1.1
Implementation Version Name	BRCONN_3.0

## 5.2. AE Specifications

### 5.2.1. Media AE - Specification

The supported Application Profiles, their Roles and the Service Class options, all defined in DICOM terminology, are listed in the following table.

**Table 59: AE Related Application Profiles, Real-World Activities, and Roles**

Supported Application Profile	Real-World Activity	Roles	SC Option
CT/MR studies on CD-R	Write Images	FSC	Interchange
	Read Images	FSR	Interchange
STD-GEN-CD	Write Images	FSC	Interchange
	Read Images	FSR	Interchange

#### 5.2.1.1. File Meta Information for the Media AE

The Application Entity title is registered into the DICOM File Meta Information header and is supported by the CD-writer (CD write option) acting as a FSC.

#### 5.2.1.2. Real-World Activities

The SOP instances provided by the RWA are written to the CD-R media and a corresponding DICOMDIR is created.

##### 5.2.1.2.1. Display Directory

When a database open action is initiated on the CD-R then the Media AE acts as an FSR using the interchange option to read the DICOMDIR of the CD or CD-R media.

This will result in an overview of the patients, studies, series and images on the Extended Brilliance Workspace screen.

##### 5.2.1.2.1.1. Media Storage Application Profile

As depicted in Table 59, the Media AE supports the RWA Display Directory for the Application Profile.

The mandatory DICOMDIR keys are required for the correct display of directory information. The display is structured according the DICOM Composite Information Model: Patient, Study, Series, and Image.

### 5.2.1.2.2. Write Images

When an image transfer to CD-R is initiated then the Media AE acts as an FSC using the interchange option to export SOP Instances from the local database to a CD-R medium.

#### 5.2.1.2.2.1. Media Storage Application Profile

As depicted in Table 59, the Media AE supports the RWA Write Images for the Application Profile.

The DICOMDIR file will be extended when new images are written. In case some attributes are not present in an image but are specified as mandatory in the DICOMDIR definition in DICOM Media, a generated value will be filled in.

#### Implementation remarks and restrictions

When writing the DICOMDIR records, key values are generated when no value of the corresponding attribute is supplied, according to the following tables.

**Table 60: Generated Keys**

Key	Tag	Generated Value
Study Keys		
Study Date	(0008,0020)	
Study Time	(0008,0030)	
Series Keys		
Series Number	(0020,0011)	1
Image Keys		
Instance Number	(0020,0013)	1

The data selected to write to the media must fit on the currently inserted media. If it does not fit, an error is generated and it is up to the operator to re-select a smaller amount of data to be written to the media. The system will not request additional media or write across multiple media.

### 5.2.1.3. DICOMDIR keys

**Table 61: Supported attributes in the DICOMDIR**

Dicom Tag	Description
0002:0001	File Meta Information Version
0002:0002	UI Media Storage Sop Class UID
0002:0003	UI Media Storage Sop Instance UID
0002:0010	UI Transfer Syntax UID
0002:0012	UI Implementation Class UID
	File Set and Directory Information
0004:1130	File Set ID
0004:1200	First Directory Record Offset
0004:1202	Last Directory Record Offset
0004:1212	File Set Consistency Flag
0004:1220	Directory Record Sequence
	Patient level

Dicom Tag	Description
0004:1400	Offset Of The Next Dir Record
0004:1410	Record In Use Flag
0004:1420	Offset Of Ref Lower Level Dir Ent
0004:1430	Directory Record Type
0010:0010	Patient's Name
0010:0020	Patient ID
	Study level
0004:1400	Offset Of The Next Dir Record
0004:1410	Record In Use Flag
0004:1420	Offset Of Ref Lower Level Dir Ent
0004:1430	Directory Record Type
0008:0020	Study Date
0008:0030	Study Time
0008:0050	Accession Number
0008:1030	Study Description
0020:000D	Study Instance UID
0020:0010	Study ID
0020:1206	Number Of Study Related Series
0020:1208	Number Of Study Related Images
	Series level
0004:1400	Offset Of The Next Dir Record
0004:1410	Record In Use Flag
0004:1420	Offset Of Ref Lower Level Dir Ent
0004:1430	Directory Record Type
0008:0060	Modality
0018:1030	Protocol Name
0020:000E	Series Instance UID
0020:0011	Series Number
0020:1209	Number of Series Related Instances
	Image level
0004:1400	Offset Of The Next Dir Record
0004:1410	Record In Use Flag
0004:1420	Offset Of Ref Lower Level Dir Ent
0004:1430	Directory Record Type
0004:1500	Referenced File ID
0004:1510	Referenced Sop Class UID In File
0004:1511	Ref Sop Instance UID In File
0004:1512	Referenced Transfer Syntax UID in FILE
0008:0008	Image Type
0008:0012	Instance Creation Date
0008:0013	Instance Creation Time
0008:0016	SOP Class UID
0008:0018	SOP Instance UID
0008:0023	Image Date
0008:0033	Image Time
0018:0010	Contrast/Bolus Agent
0018:1120	Gantry/Detector Tilt
0020:0013	Instance Number
0020:0052	Frame of Reference UID
0020:1041	Slice Location
0028:0002	Samples per Pixels

---

Dicom Tag	Description
0028:0010	Rows
0028:0011	Columns
0028:0100	Bits Allocated

#### **5.2.1.3.1. Read Images**

When an image transfer from CD or CD-R is initiated then the Media AE acts as an FSR using the interchange option to import SOP Instances from the CD or CD-R medium.

##### **5.2.1.3.1.1. Media Storage Application Profile**

As depicted in Table 59, the Media AE supports the RWA Read Images for the Application Profile.

The mandatory attributes of the DICOM images are required for the correct storage of the images in the Extended Brilliance Workspace internal image database. Optional attributes and Retired/Private attributes are stored too – if present; this is equivalent with the level 2 (Full) conformance for the Storage service class in the Network support;

### **5.3. Augmented and Private Application Profiles**

This section is used for the description of augmented and private Application Profiles.

#### **5.3.1. Augmented Application Profiles**

None.

#### **5.3.2. Private Application Profiles**

None.

### **5.4. Media Configuration**

Any configuration issues may be found in the Networking Section 4.4 Configuration.



## 6. SUPPORT OF CHARACTER SETS

Any support for character sets beyond the default character repertoire in Network and Media services shall be described here.

**Table 62: Supported DICOM Character Sets**

Character Set Description	Defined Term	ESC Sequence	ISO Registration Number	Code Element	Character Set
Single-byte Character Sets without Code Extensions					
Default repertoire	-	-	ISO-IR 6	G0	ISO 646
Latin alphabet No. 1	ISO_IR 100	-	ISO-IR 6	G0	ISO 646
		-	ISO-IR 100	G1	Supplementary set of ISO 8859

---

## 7. SECURITY

### 7.1. Security Profiles

None supported.

### 7.2. Association Level Security

None supported

### 7.3. Application Level Security

None supported

## 8. ANNEXES

### 8.1. CT IOD Contents

#### 8.1.1. Created SOP Instances

##### 8.1.1.1. General Rules

This section specifies the IODs created by the Extended Brilliance Workspace.

Abbreviations used for the IOD tables are:

COPY                    the module is copied from the source images  
 ALWAYS                the module is always present (created)  
 CONDITIONAL         the module exists under specified condition

The Extended Brilliance Workspace reflects the fact that the IOD created by the workstation are always based on some source images after the viewing/processing applied and the modified images are saved. Most of the attributes or even the whole modules (Patient, General Study, etc.) are just copied from the source images. The base of the copied attribute is the DICOM Standard.

The following table lists the modules that are always copied from the source images when the created SOP Class IOD is the same as the source SOP Class IOD:

**Table 63: Modules Copied to the Derived IODs Table**

Information Entity	Module Name	Reference	Presence of Module
Patient	Patient Module		COPY
	Clinical Trial Subject Module		COPY
Study	General Study Module		COPY
	Patient Study Module		COPY
	Clinical Trial Study Module		COPY
Series	General Series Module		ALWAYS CREATED
	Clinical Trial Series Module		COPY
Frame of Reference	Frame of Reference Module		COPY
Equipment	General Equipment Module		COPY

##### 8.1.1.2. SC Image IOD Modules

**Table 64: SC Image IOD Modules Table**

Information Entity	Module Name	Presence of Module
Patient	Patient Module	COPY
Study	General Study Module	COPY
	Patient Study Module	COPY
Series	General Series Module	ALWAYS

Information Entity	Module Name	Presence of Module
Equipment	General Equipment Module	COPY
	SC Equipment Module	ALWAYS
Image	General Image Module	ALWAYS
	Image Pixel Module	ALWAYS
	SC Image Module	ALWAYS
	Overlay Plane	CONDITIONAL - if present in the displayed image
	Modality LUT	CONDITIONAL – if Bits Stored > 8
	VOI LUT Module	CONDITIONAL – if Bits Stored > 8
	SOP Common Module	ALWAYS

### 8.1.1.3. Key Object Selection Document IOD Modules

**Table 65: Key Object Selection Document IOD Modules Table**

Information Entity	Module Name	Reference	Presence of Module
Patient	Patient Module		COPY
Study	General Study Module		COPY
	Patient Study Module		COPY
Series	Key Object Document Series Module		ALWAYS
Equipment	General Equipment Module		COPY
Document	Key Object Document		ALWAYS
	SR Document Content		ALWAYS
	SOP Common Module		ALWAYS

### 8.1.1.4. Encapsulated PDF IOD Modules

**Table 66: Encapsulated PDF IOD Modules Table**

Information Entity	Module Name	Reference	Presence of Module
Patient	Patient Module		COPY
	Specimen Identification		COPY
Study	General Study Module		COPY
	Patient Study Module		COPY
Series	Encapsulated Document Series		ALWAYS
Equipment	General Equipment Module		COPY
	SC Equipment Module		ALWAYS
Image	Encapsulated Document		ALWAYS
	SOP Common Module		ALWAYS

## Usage of Attributes from Received IODs

The following attributes must be present in the received IOD to be accepted:

**For all IODs:**

- SOP Class UID (00080016)
- Study Instance UID (0020000D)
- Series Instance UID (0020000E)

**For Image IODs:**

- Pixel Data (7FE0,0010) - size is not 0
- Rows (0028,0010)
- Columns (00280011)
- Bits Allocated (00280100)

**8.1.2. Attribute Mapping**

Not Applicable

**8.1.3. Coerced/Modified fields**

In the received IODs, the following attributes may be modified under certain conditions:

**Table 67: Modified Attributes**

Attribute	Tag	When Modified
Patient name	0010,0010	if empty will be set to "Unknown"
Patient Id	0010,0020	if empty will be set to "Unknown"
Rows	0028,0010	fixed if rows* columns doesnt match pixel data size
Sop Instance UID	0008,0018	generate new if missing

## 8.2. PET IOD Contents

### 8.2.1. Created SOP Instances

#### 8.2.1.1. General Rules

This section specifies the IODs created by the Extended Brilliance Workspace.

The tables in this section use numerous abbreviations. The following abbreviations are used in the “Presence of Modules” column:

VNAP	Value Not Always Present (attribute sent zero length if no value is present)
ANAP	Attribute Not Always Present
ALWAYS	Always Present
EMPTY	Attribute is sent without a value
NEVER	Attribute or Module is never sent

The following abbreviations are used in the “Source” column:

MWL	Attribute value source Modality Worklist
USER	Attribute value source is from User input
AUTO	Attribute value is generated automatically
MPPS	Attribute value is the same as that used for Modality Performed Procedure Step
CONFIG	Attribute value source is a configurable parameter

*Note: All dates and times are encoded in the local configured calendar and time.*

#### 8.2.1.2. PET Image IOD

**Table 68: IOD of Created PET SOP Instances**

Information Entity	Module Name	Reference	Presence of Module
Patient	Patient Module	Table 76	ALWAYS
Study	General Study Module	Table 77	ALWAYS
	Patient Study Module	Table 78	ALWAYS
Series	General Series Module	Table 79	ALWAYS
	PET Series Module	Table 89	ALWAYS
	PET Isotope	Table 90	ALWAYS
	PET Multi-Gated Acquisition		VNAP
	NM/PET Patient Orientation	Table 91	ALWAYS
Frame of Reference	Frame of Reference Module	Table 80	ALWAYS
Equipment	General Equipment Module	Table 81	ALWAYS
Image	General Image Module	Table 83	ALWAYS
	Image Plane Module	Table 84	ALWAYS
	Image Pixel Module	Table 85	ALWAYS
	PET Image Module	Table 92	ALWAYS
	VOI LUT Module		NEVER
	Overlay Plane Module		NEVER
	SOP Common Module	Table 87	ALWAYS

## 8.2.1.3. NM Image IOD

Table 69: IOD of Created NM SOP Instances

Information Entity	Module Name	Reference	Presence of Module
Patient	Patient Module	Table 76	ALWAYS
Study	General Study Module	Table 77	ALWAYS
	Patient Study Module	Table 78	ALWAYS
Series	General Series Module	Table 79	ALWAYS
	NM/PET Patient Orientation Module	Table 91	ALWAYS
Frame of Reference	Frame of Reference Module	Table 80	ALWAYS
Equipment	General Equipment Module	Table 81	ALWAYS
Image	NM Image Pixel Module	Table 93	ALWAYS
	General Image Module	Table 83	ALWAYS
	Image Pixel Module	Table 85	ALWAYS
	Multi-frame Module	Table 88	ALWAYS
	NM Multi-frame Module	Table 94	ALWAYS
	NM Image Module	Table 95	ALWAYS
	NM Isotope Module	Table 96	ALWAYS
	NM Detector Module	Table 97	ALWAYS
	NM TOMO Acquisition Module	Table 98	ALWAYS
	NM Multi-gated Acquisition Module		VNAP
	NM Phase Module		VNAP
	NM Reconstruction Module	Table 99	ALWAYS
	Overlay Plane Module		NEVER
	Multi-frame Overlay Module		NEVER
	Curve		NEVER
VOI LUT Module		NEVER	
SOP Common Module	Table 87	ALWAYS	

## 8.2.1.4. Secondary Capture Image IOD

Table 70: IOD of Created Secondary Capture SOP Instances

Information Entity	Module Name	Reference	Presence of Module
Patient	Patient Module	Table 76	ALWAYS
Study	General Study Module	Table 77	ALWAYS
	Patient Study Module	Table 78	ALWAYS
Series	General Series Module	Table 79	ALWAYS
Equipment	General Equipment Module	Table 81	ALWAYS
	SC Equipment Module	Table 82	ALWAYS
Image	General Image Module	Table 83	ALWAYS
	Image Pixel Module	Table 85	ALWAYS
	SC Image Module	Table 86	ALWAYS
	Overlay Plane Module		NEVER
	Modality LUT Module		NEVER
	VOI LUT Module		NEVER
	SOP Common Module	Table 87	ALWAYS

### 8.2.1.5. Multi-Frame Grayscale Byte Secondary Capture Image IOD

**Table 71: IOD of Created Multi-frame Grayscale Byte Secondary Capture SOP Instances**

Information Entity	Module Name	Reference	Presence of Module
Patient	Patient Module	Table 76	ALWAYS
	Clinical Trial Subject Module		NEVER
Study	General Study Module	Table 77	ALWAYS
	Patient Study Module	Table 78	ALWAYS
	Clinical Trial Study Module		NEVER
Series	General Series Module	Table 79	ALWAYS
	Clinical Trial Series Module		NEVER
Equipment	General Equipment Module	Table 81	ALWAYS
	SC Equipment Module	Table 82	ALWAYS
Image	General Image Module	Table 83	ALWAYS
	Image Pixel Module	Table 85	ALWAYS
	Multi-frame Module	Table 88	ALWAYS
	SC Image Module	Table 86	ALWAYS
	SC Multi-frame Image Module	Table 100	ALWAYS
	SC Multi-frame Vector Module	Table 101	
	VOI LUT Module		NEVER
	SOP Common Module	Table 87	ALWAYS



### 8.2.1.6. True-Color Secondary Capture Image IOD

**Table 72: IOD of Created True-Color Multi-frame Secondary Capture SOP Instances**

Information Entity	Module Name	Reference	Presence of Module
Patient	Patient Module	Table 76	ALWAYS
	Clinical Trial Subject Module		NEVER
Study	General Study Module	Table 77	ALWAYS
	Patient Study Module	Table 78	ALWAYS
	Clinical Trial Study Module		NEVER
Series	General Series Module	Table 79	ALWAYS
	Clinical Trial Series Module		NEVER
Equipment	General Equipment Module	Table 81	ALWAYS
	SC Equipment Module	Table 82	ALWAYS
Image	General Image Module	Table 83	ALWAYS
	Image Pixel Module	Table 85	ALWAYS
	Cine Module		NEVER
	Frame Pointers Module		NEVER
	Multi-frame Module	Table 88	ALWAYS
	SC Image Module	Table 86	ALWAYS
	SC Multi-frame Image Module	Table 100	ALWAYS
	SC Multi-frame Vector Module	Table 101	ALWAYS
	VOI LUT Module		NEVER
SOP Common Module	Table 87	ALWAYS	

### 8.2.1.7. RT Structure Sets IOD

**Table 73: IOD of RT Structure Sets for Created SOP Instances**

Information Entity	Module Name	Reference	Presence of Module
Patient	Patient Module	Table 76	ALWAYS
	Clinical Trial Subject Module		NEVER
Study	General Study Module	Table 77	ALWAYS
	Patient Study Module	Table 78	NEVER
	Clinical Trial Study Module		NEVER
Series	RT Series Module	Table 103	ALWAYS
	Clinical Trial Series Module		NEVER
Equipment	General Equipment Module	Table 81	ALWAYS
Structure Set	RT Structure Set Module	Table 102	ALWAYS
	ROI Contour Module	Table 74	ALWAYS
	RT ROI Observations Module	Table 75	ALWAYS
	Approval Module		NEVER
	Audio Module		NEVER
	SOP Common Module	Table 87	ALWAYS

**Table 74: RT ROI Contour Module Attributes**

Attribute Name	Tag	VR	Value	Presence of Value	Source
ROI Contour Sequence	(3006,0039)	SQ		ALWAYS	
>Referenced ROI Number	(3006,0084)	IS		ALWAYS	
>ROI Display Color	(3006,002A)	IS		ALWAYS	
>Contour Sequence	(3006,0040)	SQ		ALWAYS	
>>Contour Number	(3006,0048)	IS		NEVER	
>>Attached Contours	(3006,0049)	IS		NEVER	
>>Contour Image Sequence	(3006,0016)	SQ		ALWAYS	
>>>Referenced SOP Class UID	(0008,1150)	UI		ALWAYS	
>>>Referenced SOP Instance UID	(0008,1155)	UI		ALWAYS	
>>>Referenced Frame Number	(0008,1160)	IS		NEVER	
>>Contour Geometric Type	(3006,0042)	CS	CLOSED PLANAR	ALWAYS	
>>Contour Slab Thickness	(3006,0044)	DS		NEVER	
>>Contour Offset Vector	(3006,0045)	DS		NEVER	
>>Number of Contour Points	(3006,0046)	IS		ALWAYS	
>>Contour Data	(3006,0050)	DS		ALWAYS	

**Table 75: RT ROI Observations Module Attributes**

Attribute Name	Tag	VR	Value	Presence of Value	Source
RT ROI Observations Sequence	(3006,0080)	SQ		ALWAYS	
>Observation Number	(3006,0082)	IS		ALWAYS	
>Referenced ROI Number	(3006,0084)	IS		ALWAYS	
>ROI Observation Label	(3006,0085)	SH		NEVER	
>ROI Observation Description	(3006,0088)	ST		NEVER	
>RT ROI Interpreted Type	(3006,00A4)	CS		NEVER	
>ROI Interpreter	(3006,00A6)	PN		NEVER	
>Material ID	(300A,00E1)	SH		NEVER	

### 8.1.1.7 Common Modules

**Table 76: Common Patient Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Patient's Name	(0010,0010)	PN		ALWAYS	MWL or User
Patient ID	(0010,0020)	LO		ALWAYS	MWL or User
Patient's Birth Date	(0010,0030)	DA		ALWAYS	MWL or User
Patient's Sex	(0010,0040)	CS		ALWAYS	MWL or User
				SC IOD VNAP	
Other Patient IDs	(0010,1000)	LO		VNAP	MWL
Patient Comments	(0010,4000)	LT		VNAP	
Ethnic Group	10,2160	SH		VNAP	MWL

**Table 77: Common General Study Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Study Instance UID	(0020,000D)	UI		ALWAYS	MWL or AUTO
Study Date	(0080,0020)	DA		ALWAYS	AUTO
Study Time	(0008,0030)	TM		ALWAYS	AUTO
Referring Physician's Name	(0008,0090)	PN		VNAP	USER
Study ID	(0020,0010)	SH		ALWAYS	USER
Accession Number	(0008,0050)	SH		VNAP	MWL or USER
Study Description	(0008,1030)	LO		ALWAYS	USER
Procedure Code Sequence	(0008,1032)	SQ		VNAP	MWL

**Table 78: Common Patient Study Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Admitting Diagnosis Description	(0008,1080)	LO		NEVER	
Patient's Age	(0010,1010)	AS		NEVER	
Patient's Weight	(0010,1030)	DS		VNAP	USER
Additional Patient History	(0010,21B0)	LT		VNAP	MWL

**Table 79: Common General Series Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Modality	(0008,0060)	CS		ALWAYS	AUTO
Series Instance UID	(0020,000E)	UI		ALWAYS	AUTO
Series Number	(0020,0011)	IS		ALWAYS	AUTO
Laterality	(0020,0060)	CS		NEVER	
Series Date	(0008,0021)	DA		ALWAYS	AUTO
Series Time	(0008,0031)	TM		ALWAYS	AUTO
Performing Physician's Name	(0008,1050)	PN		NEVER	
Protocol Name	(0018,1030)	LO		ALWAYS	AUTO
Series Description	(0008,103E)	LO		ALWAYS	AUTO
Operator's Name	(0008,1070)	PN		NEVER	
Referenced Performed Procedure Step Sequence	(0008,1111)	SQ		NEVER VNAP	
>Referenced SOP Class UID	(0008,1150)	UI		NEVER VNAP	
>Referenced SOP Instance UID	(0008,1155)	UI		NEVER VNAP	
Body Part Examined	(0018,0015)	CS		NEVER	
Patient Position	(0018,5100)	CS		ALWAYS	AUTO
Smallest Pixel Value in Series	(0028,0108)	SS		NEVER	
Largest Pixel Value in Series	(0028,0109)	SS		NEVER	
Request Attributes Sequence	(0040,0275)	SQ		NEVER VNAP	MWL
>Requested Procedure ID	(0040,1001)	SH		NEVER VNAP	MWL
>Scheduled Procedure Step ID	(0040,0009)	SH		NEVER VNAP	MWL
>Scheduled Procedure Step Description	(0040,0007)	LO		NEVER VNAP	MWL
>Scheduled Protocol Code Sequence	(0040,0008)	SQ		NEVER VNAP	MWL
Performed Procedure Step ID	(0040,0253)	SH		NEVER VNAP	MWL
Performed Procedure Step Start Date	(0040,0244)	DA		NEVER VNAP	MWL
Performed Procedure Step Start Time	(0040,0245)	TM		NEVER VNAP	MWL
Performed Procedure Step Description	(0040,0254)	LO		NEVER VNAP	MWL
Performed Protocol Code Sequence	(0040,0260)	SQ		NEVER VNAP	MWL
Comments on the Performed Procedure Step	(0040,0280)	LO		NEVER VNAP	MWL

**Table 80: Common Frame of Reference Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Frame of Reference UID	(0020,0052)	UI		ALWAYS	AUTO
Position Reference Indicator	(0020,1040)	LO		VNAP	

**Table 81: Common General Equipment Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Manufacturer	(0008,0070)	LO	Philips Medical Systems	ALWAYS	AUTO
Institution Name	(0008,0080)	LO		ALWAYS	AUTO
Institution Address	(0008,0081)	ST		NEVER	
Station Name	(0008,1010)	SH		ALWAYS	AUTO
Institutional Department Name	(0008,1040)	LO		NEVER	
Manufacturer's Model Name	(0008,1090)	LO		VNAP	
Device Serial Number	(0018,1000)	LO		ALWAYS	AUTO
Software Version	(0018,1020)	LO		ALWAYS	AUTO
Spatial Resolution	(0018,1050)	DS		NEVER	
Date of Last Calibration	(0018,1200)	DA		NEVER	
Time of Last Calibration	(0018,1201)	TM		NEVER	
Pixel Padding Value	(0028,0120)	US		NEVER	

**Table 82: Common SC Image Equipment Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Conversion Type	(0008,0064)	CS	WSD	ALWAYS	
Modality	(0008,0060)	CS		ALWAYS	AUTO
Secondary Capture Device ID	(0018,1010)	LO		ALWAYS	AUTO
Secondary Capture Device Manufacturer	(0018,1016)	LO		ALWAYS	AUTO
Secondary Capture Device Manufacturer's Model Name	(0018,1018)	LO		ALWAYS	AUTO
Secondary Capture Device Software Version	(0018,1019)	LO		ALWAYS	AUTO
Video Image Format Acquired	(0018,1022)	SH		NEVER	
Digital Image Format Acquired	(0018,1023)	LO		NEVER	

**Table 83: Common General Image Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Instance Number	(0020,0013)	IS		ALWAYS	AUTO
Patient Orientation	(0020,0020)	CS		NEVER	
Content Date	(0008,0023)	DA		ALWAYS	AUTO
Content Time	(0008,0033)	TM		ALWAYS	AUTO
Image Type	(0008,0008)	CS		ALWAYS VNAP	AUTO
Acquisition Number	(0020,0012)	IS		NEVER VNAP	
Acquisition Date	(00080022)	DA		ALWAYS	AUTO
Acquisition Time	(0008,0032)	TM		ALWAYS	AUTO
Acquisition Datetime	(0008,0024)	DT		NEVER	
Referenced Image Sequence	(0008,1140)	SQ		NEVER	
>Referenced SOP Class UID	(0009,1150)	UI		NEVER	
>Referenced SOP Instance UID	(0008,1151)	UI		NEVER	
>Referenced Frame Number	(0008,1160)	IS		NEVER	
>Purpose of Reference Code Sequence	(0040,A170)	SQ		NEVER	
Derivation Description	(0008,2111)	ST		NEVER	
Derivation Code Sequence	(0008,9215)	SQ		NEVER	
Source Image Sequence	(0008,2112)	SQ		NEVER	
Referenced Waveform Sequence	(0008,113A)	SQ		NEVER	
Images in Acquisition	(0020,1002)	IS		NEVER	
Image Comments	(0020,4000)	LT		VNAP	AUTO
Quality Control Image	(0028,0300)	CS		NEVER	
Burned in Annotation	(0028,0301)	CS		NEVER VNAP	
Lossy Image Compression	(0028,2110)	DS		NEVER	
Lossy Image Compression Ratio	(0088,0200)	DS		NEVER	
Icon Image Sequence	(0088,0200)	SQ		NEVER	
Presentation LUT Shape	(2050,0020)	CS		NEVER	

**Table 84: Common Image Plane Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Pixel Spacing	(0028,0030)	DS		ALWAYS	AUTO
Image Orientation (Patient)	(0020,0037)	DS		ALWAYS	AUTO
Image Position	(0020,0032)	DS		ALWAYS	AUTO
Slice Thickness	(0018,0050)	DS		ALWAYS	AUTO
Slice Location	(0020,1041)	DS		VNAP	

**Table 85: Common Image Pixel Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Pixel Data	(7FEO,0010)	OW/ OB		ALWAYS	AUTO
Samples per Pixel	(0028,0002)	US		ALWAYS	AUTO
Photometric Interpretation	(0028,0004)	CS		ALWAYS	AUTO
Rows	(0028,0010)	US		ALWAYS	AUTO
Columns	(0028,0011)	US		ALWAYS	AUTO
Bits Allocated	(0028,0100)	US		ALWAYS	AUTO
Bits Stored	(0028,0101)	US		ALWAYS	AUTO
High Bit	(0028,0102)	US		ALWAYS	AUTO
Pixel Representation	(0028,0103)	US		ALWAYS	AUTO
Planar Configuration	(0028,0006)	US		NEVER VNAP	
Pixel Aspect Ratio	(0028,0034)	IS		NEVER VNAP	
Smallest Image Pixel Value	(0028,0106)	US		ALWAYS VNAP	AUTO
Largest Image Pixel Value	(0028,0107)	US		ALWAYS VNAP	AUTO
Red Palette Color Lookup Table Descriptor	(0028,1101)	US		NEVER	
Green Palette Color Lookup Table Descriptor	(0028,1102)	US		NEVER	
Blue Palette Color Lookup Table Descriptor	(0028,1103)	US		NEVER	
Red Palette Color Lookup Table Data	(0028,1201)	OW		NEVER	
Green Palette Color Lookup Table Data	(0028,1202)	OW		NEVER	
BLUE Palette Color Lookup Table Data	(0028,1203)	OW		NEVER	

**Table 86: Common SC Image Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Date of Secondary Capture	(0018,1012)	DA		ALWAYS	AUTO
Time of Secondary Capture	(0018,1014)	TM		ALWAYS	AUTO

**Table 87: Common SOP Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
SOP Class UID	(0008,0016)	UI		ALWAYS	AUTO
SOP Instance UID	(0008,0018)	UI		ALWAYS	AUTO
Specific Character Set	(0008,0005)	CS		NEVER	
Instance Creation Date	(0008,0012)	DA		NEVER VNAP	
Instance Creation Time	(0008,0013)	TM		NEVER VNAP	
Instance Creator UID	(0008,0014)	UI		NEVER	
Scheme Identification Sequence	(0008,0110)	SQ		NEVER	
Timezone Offset From UTC	(0008,0201)	SH		NEVER	
Contributing Equipment Sequence	(0008,A001)	SQ		NEVER	
Instance Number	(0020,0013)	IS		ALWAYS	AUTO
SOP Instance Status	(0100,0410)	CS		NEVER	
SOP Authorization Date and Time	(0100,0420)	DT		NEVER	
SOP Authorization Comment	(0100,0424)	LT		NEVER	
Authorization Equipment Certification Number	(0100,0426)	LO		NEVER	
Encrypted Attributes Sequence	(0040,0500)	SQ		NEVER	

**Table 88: Common Multi-frame Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Number of Frames	(0028,0008)	IS		ALWAYS	AUTO
Frame Increment Pointer	(0028,0009)	AT		ALWAYS	AUTO



## 8.2.1.8. PET Modules

Table 89: PET Series Module for Created SOP Instances

Attribute Name	Tag	VR	Value	Presence of Value	Source
Series Date	(0008,0021)	DA		ALWAYS	AUTO
Series Time	(0008,0031)	TM		ALWAYS	AUTO
Units	(0054,1001)	CS	CNTS	ALWAYS	AUTO
Counts Source	(0054,1002)	CS		ALWAYS	AUTO
Series Type	(0054,1000)	CS		ALWAYS	AUTO
Reprojection Method	(0054,1004)	CS		NEVER	
Number of R-R Intervals	(0054,0061)	US		NEVER VNAP	
Number of Time Slots	(0054,0071)	US		NEVER VNAP	
Number of Time Slices	(0054,0101)	US		VNAP	AUTO
Number of Slices	(0054,0081)	US		ALWAYS	AUTO
Corrected Image	(0028,0051)	CS		ALWAYS	AUTO
Randoms Correction Method	(0054,1100)	CS		ALWAYS	AUTO
Attenuation Correction Method	(0054,1101)	LO		ALWAYS	AUTO
Scatter Correction Method	(0054,1105)	LO		ALWAYS	AUTO
Decay Correction	(0054,1102)	CS		ALWAYS	AUTO
Reconstruction Diameter	0018,1100)	DS		ALWAYS	AUTO
Convolution Kernel	(0018,1210)	SH		NEVER	
Reconstruction Method	(0054,1103)	LO		ALWAYS	AUTO
Detector Lines of Response Used	(0054,1104)	LO		NEVER	
Acquisition Start Condition	(0018,0073)	CS		NEVER	
Acquisition Start Condition Data	(0018,0074)	IS		NEVER	
Acquisition Termination Condition	(0018,0071)	CS		NEVER	
Acquisition Termination Condition Data	(0018,0075)	IS		NEVER	
Field of View Shape	(0018,1147)	CS	CYLINDRICAL RING	ALWAYS	AUTO
Field of View Dimensions	(0018,1149)	IS		ALWAYS	AUTO
Gantry/Detector Tilt	(0018,1120)	DS		NEVER	
Gantry/Detector Slew	(0018,1121)	DS		NEVER	
Type of Detector Motion	(0054,0202)	CS	NONE	ALWAYS	AUTO
Collimator Type	(0018,1181)	CS	NONE	ALWAYS	AUTO
Collimator/Grid Name	(0018,1180)	SH		NEVER	
Axial Acceptance	(0054,1200)	DS		NEVER	
Axial Mash	(0054,1201)	IS		NEVER	
Transverse Mash	(0054,1202)	IS		NEVER	
Detector Element Size	(0054,1203)	DS		NEVER	
Coincidence Window Width	(0054,1210)	DS		NEVER	
Energy Window Range Sequence	(0054,0013)	SQ		NEVER	
Secondary Counts Type	(0054,1220)	CS		NEVER	

**Table 90: PET Isotope Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Radiopharmaceutical Information Sequence	(0054,0016)	SQ		ALWAYS	AUTO
>Radionuclide Code Sequence	(0054,0300)	SQ		ALWAYS	AUTO
>Radiopharmaceutical Route	(0018,1070)	LO		NEVER	
>Administration Route Code Sequence	(0054,0302)	SQ		NEVER	
>Radiopharmaceutical Volume	(0018,1071)	DS		NEVER	
>Radiopharmaceutical Start Time	(0018,1072)	TM		ALWAYS	AUTO
>Radiopharmaceutical Stop Time	(0018,1073)	TM		ALWAYS	AUTO
>Radionuclide Total Dose	(0018,1074)	DS		ALWAYS	AUTO
>Radionuclide Half Life	(0018,1075)	DS		ALWAYS	AUTO
>Radionuclide Positron Fraction	(0018,1076)	DS		NEVER	
>Radiopharmaceutical Specific Activity	(0018,1077)	DS		NEVER	
>Radiopharmaceutical	(0018,0031)	LO		NEVER VNAP	
>Radiopharmaceutical Code Sequence	(0054,0304)	SQ		NEVER VNAP	
Intervention Drug Information Sequence	(0018,0026)	SQ		NEVER	

**Table 91: NM/PET Patient Orientation Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Patient Orientation Code Sequence	0054,0410	SQ		ALWAYS	AUTO
Patient Orientation Modifier Code Sequence	0054,0412	SQ		ALWAYS	AUTO
Patient Gantry Relationship Code Sequence	0054,0104	SQ		ALWAYS	AUTO

Table 92: PET Image Module for Created SOP Instances

Attribute Name	Tag	VR	Value	Presence of Value	Source
Image Type	(0008,0008)	CS		ALWAYS	AUTO
Samples per Pixel	(0028,0002)	US		ALWAYS	AUTO
Photometric Interpretation	(0028,0004)	CS		ALWAYS	AUTO
Bits Allocated	(0028,0100)	US		ALWAYS	AUTO
Bits Stored	(0028,0101)	US		ALWAYS	AUTO
High Bit	(0028,0102)	US		ALWAYS	AUTO
Rescale Intercept	(0028,1052)	DS		ALWAYS	AUTO
Rescale Slope	(0028,1053)	DS		ALWAYS	AUTO
Frame Reference Time	(0054,1300)	DS		ALWAYS	AUTO
Trigger Time	(0018,1060)	DS		NEVER VNAP	
Frame Time	(0018,1063)	DS		NEVER VNAP	
Low R-R Value	(0018,1081)	IS		NEVER VNAP	
High R-R Value	(0018,1082)	IS		NEVER VNAP	
Lossy Image Compression	(0028,2110)	CS		NEVER	
Image Index	(0054,1330)	US		ALWAYS	AUTO
Acquisition Date	(0008,0022)	DA		ALWAYS	AUTO
Acquisition Time	(0008,0032)	TM		ALWAYS	AUTO
Actual Frame Duration	(0018,1242)	IS		ALWAYS	AUTO
Nominal Interval	(0018,1062)	IS		NEVER	
Intervals Acquired	(0018,1083)	IS		NEVER VNAP	
Intervals Rejected	(0018,1084)	IS		NEVER VNAP	
Primary (Prompts) Counts Accumulated	(0054,1310)	IS		NEVER	
Secondary Counts Accumulated	(0054,1311)	IS		NEVER	
Slice Sensitivity Factor	(0054,1320)	DS		NEVER	
Decay Factor	(0054,1321)	DS		NEVER	
Dose Calibration Factor	(0054,1322)	DS		NEVER	
Scatter Fraction Factor	(0054,1323)	DS		NEVER	
Dead Time Factor	(0054,1324)	DS		NEVER	
Referenced Overlay Sequence	(0008,1130)	SQ		NEVER	
Referenced Curve Sequence	(0008,1145)	SQ		NEVER	
Anatomic Region Sequence	(0008,2218)	SQ		NEVER	
Primary Anatomic Structure Sequence	(0008,2228)	SQ		NEVER	

**Table 93: NM Image Pixel Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Samples per Pixel	(0028,0002)	US		ALWAYS	AUTO
Photometric Interpretation	(0028,0004)	CS		ALWAYS	AUTO
Bits Allocated	(0028,0100)	US		ALWAYS	AUTO
Bits Stored	(0028,0101)	US		ALWAYS	AUTO
High Bit	(0028,0102)	US		ALWAYS	AUTO
Pixel Spacing	(0028,0030)	DS		ALWAYS	AUTO

**8.2.1.9. NM Modules****Table 94: NM Multi-frame Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Frame Increment Pointer	(0028,0009)	AT		ALWAYS	AUTO
Energy Window Vector	(0028,0010)	US		NEVER VNAP	
Number of Energy Windows	(0028,0011)	US		ALWAYS	AUTO
Detector Vector	(0054,0020)	US		NEVER VNAP	
Number of Detectors	(0054,0021)	US		ALWAYS	AUTO
Phase Vector	(0054,0030)	US		NEVER VNAP	
Number of Phases	(0054,0031)	US		ALWAYS	
Rotation Vector	(0054,0050)	US		NEVER VNAP	
Number of Rotations	(0054,0051)	US		ALWAYS	AUTO
R-R Interval Vector	(0054,0060)	US		NEVER VNAP	
Number of R-R Intervals	(0054,0061)	US		NEVER VNAP	
Time Slot Vector	(0054,0070)	US		NEVER VNAP	
Number of Time Slots	(0054,0071)	US		NEVER VNAP	
Slice Vector	(0054,0080)	US		ALWAYS	AUTO
Number of Slices	(0054,0081)	US		ALWAYS	AUTO
Angular View Vector	(0054,0090)	US		NEVER	
Time Slice Vector	(0054,0100)	US		NEVER VNAP	

**Table 95: NM Image Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Image Type	(0008,0008)	CS		ALWAYS	AUTO
Image ID	(0054,0400)	SH		NEVER	
Lossy Image Compression	(0028,2110)	CS		NEVER	
Counts Accumulated	(0018,0070)	IS		ALWAYS	AUTO
Acquisition Termination Condition	(0018,0071)	CS		NEVER	
Table Height	(0018,1130)	DS		NEVER	
Table Traverse	(0018,1131)	DS		NEVER	
Actual Frame Duration	(0018,1242)	IS		NEVER VNAP	
Count Rate	(0018,1243)	IS		NEVER	
Processing Function	(0018,5020)	LO		NEVER	
Corrected Image	(0028,0051)	CS		ALWAYS	AUTO
Whole Body Technique	(0018,1301)	CS		NEVER	
Scan Velocity	(0018,1300)	DS		NEVER	
Scan Length	(0018,1302)	IS		NEVER	
Referenced Overlay Sequence	(0008,1130)	SQ		NEVER	
Referenced Curve Sequence	(0008,1145)	SQ		NEVER	
Trigger Source or Type	(0018,1061)	LO		NEVER	
Anatomic Region Sequence	(0008,2218)	SQ		NEVER	
Primary Anatomical Structure Sequence	(0008,2228)	SQ		NEVER	

**Table 96: NM Isotope Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Energy Window Information Sequence	(0054,0012)	SQ		ALWAYS	AUTO
>Energy Window Name	(0054,0018)	SH		NEVER	
>Energy Window Range Sequence	(0054,0013)	SQ		NEVER	
Radiopharmaceutical Information Sequence	(0054,0015)	SQ		ALWAYS	AUTO
>Radionuclide Code Sequence	(0054,0300)	SQ		ALWAYS	AUTO
>Radiopharmaceutical Route	(0018,1070)	LO		NEVER	
>Administration Route Code Sequence	(0054,0302)	SQ		NEVER	
>Radiopharmaceutical Volume	(0018,1071)	DS		NEVER	
>Radiopharmaceutical Start Time	(0018,1072)	TM		ALWAYS	AUTO
>Radiopharmaceutical Stop Time	(0018,1073)	TM		NEVER	
>Radionuclide Total Dose	(0018,1074)	DS		ALWAYS	AUTO
>Calibration Data Sequence	(0054,0306)	SQ		NEVER	
>Radiopharmaceutical	(0018,0031)	LO		NEVER VNAP	
>Radiopharmaceutical Code Sequence	(0054,0304)	SQ		NEVER VNAP	
Intervention Drug Information Sequence	(0018,0026)	SQ		NEVER	

**Table 97: NM Detector Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Detector Information Sequence	(0054,0022)	SQ		ALWAYS	AUTO
>Collimator/Grid Name	(0018,1180)	SH		NEVER	
>Collimator Type	(0018,1181)	CS	NONE	ALWAYS	AUTO
>Field of View Shape	(0018,1147)	CS	CYLINDRICAL RING	ALWAYS	AUTO
>Field of View Dimensions (s)	(0018,1149)	IS		ALWAYS	AUTO
>Focal Distance	(0018,1182)	IS		VNAP	AUTO
>X Focus Center	(0018,1183)	DS		NEVER	
>Y Focus Center	(0018,1184)	DS		NEVER	
>Zoom Center	(0028,0032)	DS		NEVER	
>Zoom Factor	(0028,0031)	DS		NEVER	
>Center of Rotation Offset	(0018,1145)	DS		NEVER	
>Gantry/Detector Tilt	(0018,1120)	DS		NEVER	
>Distance Source to Detector	(0018,1110)	DS		NEVER	
>Start Angle	(0054,0200)	DS		NEVER	
>Radial Position	(0018,1142)	DS		NEVER	
>Image Orientation (Patient)	(0020,0037)	DS		ALWAYS	AUTO
>Image Position (Patient)	(0020,0032)	DS		ALWAYS	AUTO
>View Code Sequence	(0054,0220)	SQ		VNAP	AUTO
>>View Modifier Code Sequence	(0054,0222)	SQ		NEVER	

**Table 98: NM TOMO Acquisition Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Rotation Information Sequence	(0054,0052)	SQ		VNAP	AUTO
Type of Detector Motion	(0054,0202)	CS		NEVER	

**Table 99: NM Reconstruction Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Spacing Between Slices	(0018,0088)	DS		ALWAYS	AUTO
Reconstruction Diameter	(0018,1100)	DS		ALWAYS	AUTO
Convolution Kernel	(0018,1210)	SH		NEVER	
Slice Thickness	(0018,0050)	DS		ALWAYS	AUTO
Slice Location	(0020,1041)	DS		NEVER VNAP	

### 8.2.1.10. Secondary Capture Modules

**Table 100: SC Multi-frame Image Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Burned in Annotation	(0028,0301)	CS		ALWAYS	AUTO
Presentation LUT Shape	(2050,0020)	CS		NEVER	
Illumination	(2010,015E)	US		NEVER	
Reflected Ambient Light	(2010,0160)	US		NEVER	
Rescale Intercept	(0028,1052)	DS		NEVER	
Rescale Slope	(0028,1053)	DS		NEVER	
Rescale Type	(0028,1054)	LO		NEVER	
Frame Increment Pointer	(0028,0009)	AT		ALWAYS	
Nominal Scanned Pixel Spacing	(0018,2010)	DS		NEVER	
Digitalizing Device Transport Direction	(0018,2020)	CS		NEVER	
Rotation of Scanned Film	(0018,2030)	DS		NEVER	

**Table 101: SC Multi-frame Vector Module for Created SOP Instances**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Frame Time Vector	(0018,1065)	DS		NEVER	AUTO
Page Number Vector	(0018,2001)	SH		ALWAYS	
Frame Label Vector	(0018,2002)	SH		NEVER	
Frame Primary Angle Vector	(0018,2003)	DS		NEVER	
Frame Secondary Angle Vector	(0018,2004)	DS		NEVER	
Slice Location Vector	(0018,2005)	DS		NEVER	
Display Window Label Vector	(0018,2006)	SH		NEVER	

## 8.2.1.11. RT Structure Modules

Table 102: RT Structure Sets for Created SOP Instances

Attribute Name	Tag	VR	Value	Presence of Value	Source
Structure Set Label	(3006,0002)	SH		ALWAYS	AUTO
Structure Set Name	(3006,0004)	LO		NEVER	
Structure Set Description	(3006,0006)	ST		NEVER	
Instance Number	(0020,0013)	IS		ALWAYS	
Structure Set Date	(3006,0008)	PA		ALWAYS	
Structure Set Time	(3006,0009)	TM		ALWAYS	
Referenced Frame of Reference Sequence	(3006,0010)	SQ		ALWAYS	
>Frame of Reference UID	(0020,0052)	UI		ALWAYS	
>Frame of Reference Relationship Sequence	(3006,00C0)	SQ		NEVER	
>RT Referenced Study Sequence	(3006,0012)	SQ		ALWAYS	
>>Referenced SOP Class UID	(0008,1150)	UI		ALWAYS	
>>Referenced SOP Instance UID	(0008,1155)	UI		ALWAYS	
>>RT Referenced Series Sequence	(3006,0014)	SQ		ALWAYS	
>>>Series Instance UID	(0020,000E)	UI		ALWAYS	
>>>Contour Image Sequence	(3006,0016)	SQ		ALWAYS	
>>>>Referenced SOP Class UID	(0008,1150)	UI		ALWAYS	
>>>>Referenced SOP Instance UID	(0008,1155)	UI		ALWAYS	
>>>>Referenced Frame Number	(0008,1160)	IS		NEVER	
Structure Set ROI Sequence	(3006,0020)	SQ		ALWAYS	
>ROI Number	(3006,0022)	IS		ALWAYS	
>Referenced Frame of Reference UID	(3006,0024)	UI		ALWAYS	
>ROI Name	(3006,0026)	LO		ALWAYS	
>ROI Description	(3006,0028)	ST		NEVER	
>ROI Volume	(3006,002C)	DS		ALWAYS	
>ROI Generation Algorithm	(3006,0036)	LO MAN UAL		ALWAYS	
>ROI Generation Description	(3006,0038)	LO		NEVER	



**Table 103: RT Series Module Attributes**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Modality	(0008,0060)	CS		ALWAYS	
Series Instance UID	(0020,000E)	UI		ALWAYS	
Series Number	(0020,0011)	IS		ALWAYS	
Series Description	(0008,103E)	LO		ALWAYS	
Referenced Performed Procedure Step Sequence	(0008,1111)	SQ		NEVER	
Request Attributes Sequence	(0040,0275)	SQ		NEVER	
Performed Procedure Step ID	(0040,0253)	SH		NEVER	
Performed Procedure Step Start Date	(0040,0244)	DA		NEVER	
Performed Procedure Step Start Time	(0040,0245)	TM		NEVER	
Performed Procedure Step Description	(0040,0254)	LO		NEVER	
Performed Protocol Sequence	(0040,0260)	SQ		NEVER	

### 8.2.2. Usage of Attributes from Received IODs

The local database, remote query, and directory browsers make use of the conventional identification attributes to distinguish patients, studies, series, and instances. In particular, if two patients have the same value for Patient ID, they will be treated as the same in the browser and the local database.

### 8.2.3. Attribute Mapping

Attribute Mapping is not applicable.

### 8.2.4. Coerced/Modified Fields

No coercion is performed.

### 8.3. Data Dictionaries

The Export software provides Standard Extended conformances to the DICOM PET SOP Class. The additional Private data elements that may be included have group number 0x7053. These elements may contain Gemini and Allegro specific information that could not be encoded in the standard PET IOD, and would be meaningless for non-Gemini and non-Allegro systems. However, some receiving systems may need to be informed of the VR for these private elements in order to properly receive and store them. The following table shows the VR for each of these elements.

**Table 104: Private Elements for PET Images**

Tag	VR	Meaning	VM
7053,0010	LO	Private Creator Data element	1
7053,1000	DS	SUV Scale Factor. This value only applies when Units (0054,1001) is equal to CNTS. The SUV Scale Factor is used to convert the pixel data from counts to an SUV value. This is done by using the following formula: $\text{SUV Value} = ((\text{SV} * m) + b) * f$ where SV = original stored pixel value m = Rescale Slope (0028,1053) b = Rescale Intercept (0028,1052) f = SUV Scale Factor (7053, 1000)  If the SUV Scale Factor is 0.0, then the pixel data cannot be converted from counts to an SUV value.	1
7053,1001	OB	Private	1
7053,1002	OB	Private	1
7053,1003	ST	Original image file name	1
7053,1009	DS	Activity Concentration Scale Factor. This value only applies when Units (0054,1001) is equal to CNTS. The Activity Concentration Scale Factor is used to convert the pixel data from counts to Activity Concentration (in Bq/ml). This is done by using the following formula: $\text{Activity Concentration Value} = ((\text{SV} * m) + b) * f$ where SV = original stored pixel value m = Rescale Slope (0028,1053) b = Rescale Intercept (0028,1052) f = Activity Concentration Scale Factor (7053, 1009)  If the Activity Concentration Scale Factor is 0.0, then the pixel data cannot be converted from counts to Activity Concentration.	1

The Private Creator Data Element [7053,0010], which is used to reserve these private data elements, has value "Philips PET Private Group."

**Table 105: Private Elements for Secondary Capture Images**

Tag	VR	Meaning	VM
7053,0010	LO	Private Creator Data element	1
7053,1003	ST	Original image file name	1

**Table 106: Private Elements for PET Raw Data**

Tag	VR	Meaning
7053,0010	LO	Private Creator Data Element
7053,1007	SQ	Acquisition File Sequence
> 7053,1003	LO	File Name
> 7053,100F	UL	Segment Size
> 7053,1010	US	Segment Number
> 7053,1011	US	Number of Segments
> 7053,1012	SQ	File Data Sequence
>> 7053,1004	OB	File Data

## 8.4. Coded Terminology and Templates

### 8.4.1. GEMINI TF Templates

**Table 107: Used Templates**

Template Name	Template ID
NM Acquisition Context	TID 3470

### 8.4.2. Content Groups

**Table 108: Content groups**

Content groups Name	Content ID
Patient Orientation	CID 19
Patient Orientation Modifier	CID 20
Patient Gantry Relationship	CID 21
PET Radionuclide	CID 4020
PET Radiopharmaceuticals	CID 4021
Route of Administration	CID 11
Nuclear Medicine Projections	CID 26
NM Procedural State Values	CID 3101

### 8.4.3. PET Coded Terminology

**Table 109: PET Coded Terminology**

Tag	Name	Content ID	Configurable
0054,0300	Radionuclide Code Sequence	CID 18	NO
0054,0220	View Code Sequence	CID 26	NO
0054,0410	Patient Orientation Code Sequence	CID 19	NO
0054,0412	Patient Orientation Modifier Code Sequence	CID 20	NO
0054,0414	Patient Gantry Relationship Code Sequence	CID 21	NO
0040,A168	Concept Code Sequence	CID 3101	NO

**8.5. Grayscale Image Consistency**

Not applicable.

**8.6. Standard Extended/Specialized/Private SOPs**

No Specialized or Private SOP Classes are supported.

**8.7. Private Transfer Syntaxes**

No Private Transfer Syntaxes are supported