


Exam
Room View



Click and drag mouse over image to pan around the room

Control
Room View

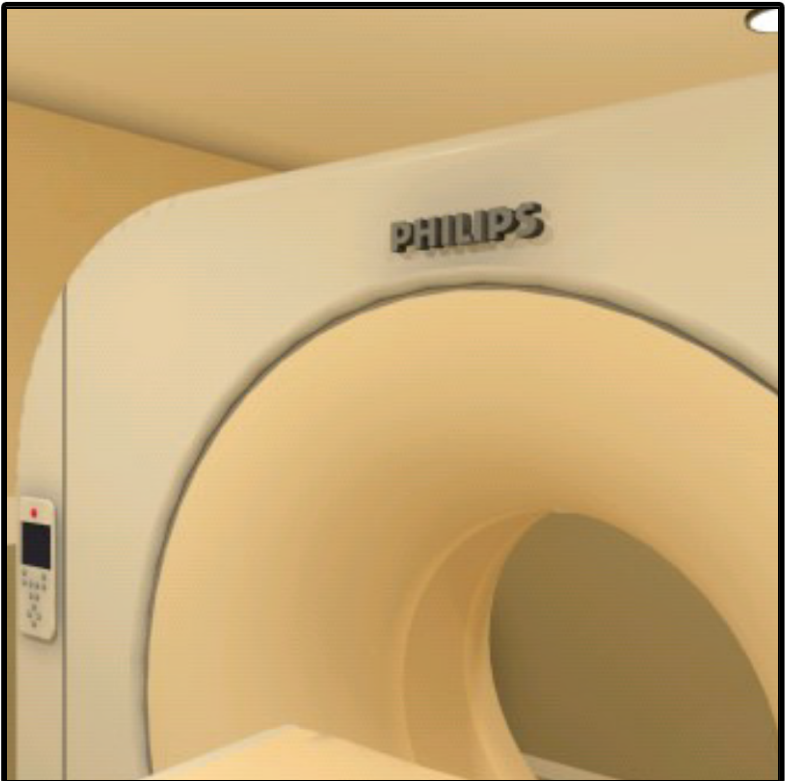

Computed
Tomography
Video




Play



Stop

MX I 6-slice CT





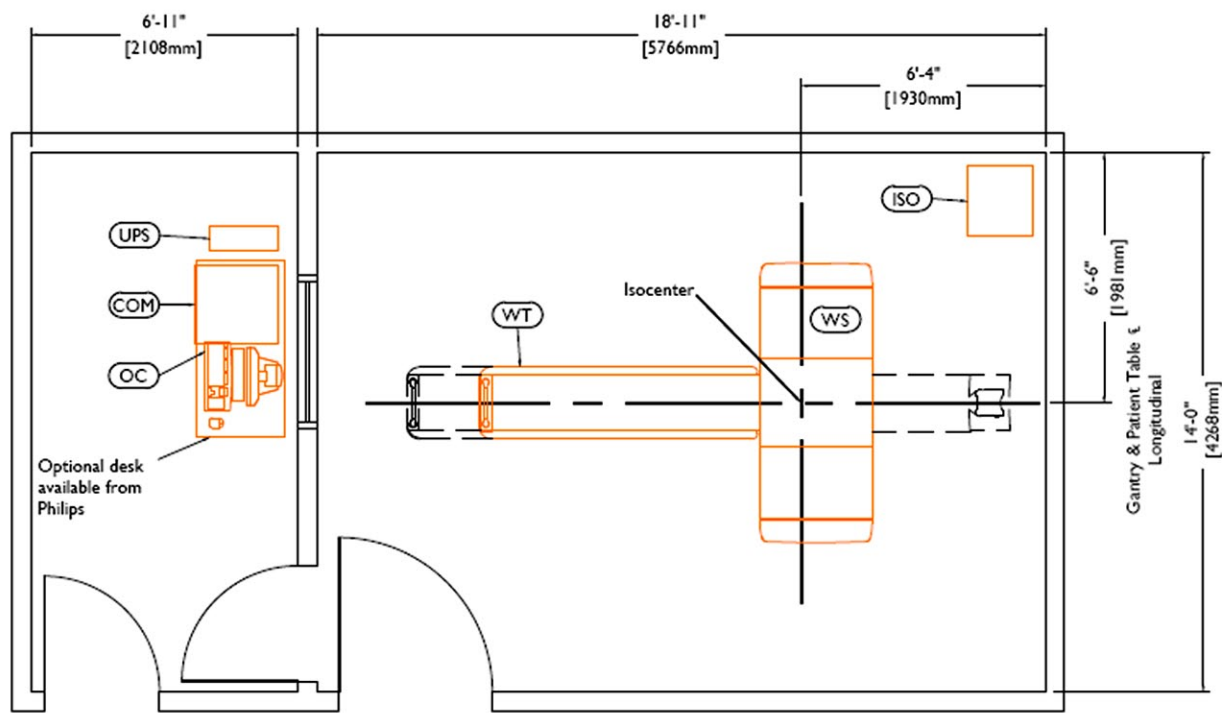

Equipment Layout

Recommended Ceiling Height: 8'-0" (2438mm)

Minimum Ceiling Height: 7'-6" (2286mm)

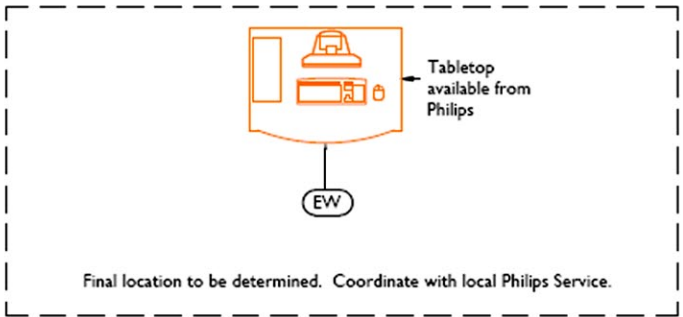

| Equipment Legend | | | | |
|---|---|--------------------|-------------------------|--|
| A Furnished and installed by Philips B Furnished by customer/contractor and installed by customer/contractor C Installed by customer/contractor D Furnished by Philips and installed by contractor E Existing F Future G Optional item furnished by Philips | | | | |
| Equipment Designation | | | | |
| Description | | Weight lbs [kg] | Heat Load Btu/hr [W] | |
| A | WS MX I 6-Slice CT Scanner Gantry | 4078 [1850] | 17075 [5004] | |
| A | WT Patient Table | 756 [343] | | |
| A | OC Operators Console | 25 [11] | 2561 [751] | |
| A | COM Computer Rack (under desk) | 331 [150] | | |
| G | ISO LM Isolation Transformer Power Unit | 604 [274] | 2210 [648] | |
| G | UPS Console UPS | 123 [56] | 375 [110] | |
| G | EW Extended Brilliance Workspace | 90 [41] | 1000 [293] | |

General System Requirements

Environmental

Operating temperature range within the CT Exam Room is 64°-75° F (18°-24° C) [ideal stable room temperature setting: 72° F (22° C)] at 30% to 60% relative humidity (non-condensing). Operating temperature change per hour throughout the CT Exam Room must not exceed 7.5° F (4.1° C).

Operating temperature range throughout the CT Suite is 64°-82° F (18°-28° C) [ideal stable room temperature setting: 72° F (22° C)] at 35% to 70% relative humidity (non-condensing). Operating temperature change per hour throughout the CT suite must not exceed 9° F (5° C).

The above conditions must be maintained at all times including overnight, weekends, and holidays. Heat output in one area of the CT Suite must not affect temperature and humidity in other areas. It is strongly recommended that any definable areas within the suite, i.e., equipment closets, control areas, etc. (if applicable), be individually environmentally controlled as required to meet the ambient ranges specified.

Power

Supply Configuration:

3 phase Delta, 4 wire power, (L1, L2, L3, PE) to Philips LM Isolation Transformer Power Unit

Nominal Line Voltage:

200-480 VAC (+/- 10%), 50/60 Hz (+/- 1 Hz)

Branch Power Requirement:

75 kVA (nominal),
65 kVA (maximum momentary power)

Remote Service Diagnostics

Medical Imaging equipment to be installed by Philips is equipped with a service diagnostic feature which allows for remote and on-site service diagnostics. To establish this feature, a RJ45 type Ethernet 10/100/1000 Mbit network connector must be installed. Access to customer's network via their remote access server is needed for Remote Service Network (RSN) connectivity. All costs with this feature are the responsibility of the customer.