


| | | | |
|-------------------------------|-----------------------|-------------------------|--|
| Product name: | dS HeadNeck coil 3.0T | | |
| Identification code(s) | 4598 000 9799x | | |
| Total weight (in Kg) | 3.8 Kg | | |
| Producer /Manufacturer | Name company: | Philips Healthcare Best | |
| | Address: | Veenpluis 4-6 | |
| | Zip code: | 5680DA Best | |
| | Country: | The Netherlands | |
| | Electronic info: | NVC HeadNeck 3.0T | |

| Recycle info | Substances: | Location |
|--|---|-----------------|
| Special attention  | Items: | |
| | 26 pcb assemblies and one flexfoil pcb assembly | Figure 1 |
| | 2 so-called RXE modules: 45221330827x or 45980004622x (containing pcb assy) | Figure 2 |
| | | |
|  Batteries <i>To be removed</i> | Type: | Location |
| | No batteries present. | |
| | | |
| | | |
| | | |
| Hazardous  To be removed | | Location |
| | SMP connectors (80 total) contain BeCu | Figure 3 |
| | | |
| | | |
|  Fluids / Gases | Items: | Location |
| | No fluids and/or gases present. | |
| | | |
| | | |

| | | | | | |
|---------|------------------------|--------------|----------------|-------------|----------------------|
| Name: | WEEE NVC HeadNeck 3.0T | 12NC: | DMR152840 | Version: 00 | Doc.Date: 2012-07-31 |
| Author: | | Pag.: 1 of 4 | Group No: 5790 | Section: - | Status: see Agile |

Locations as mentioned in the Passport (Picture information)

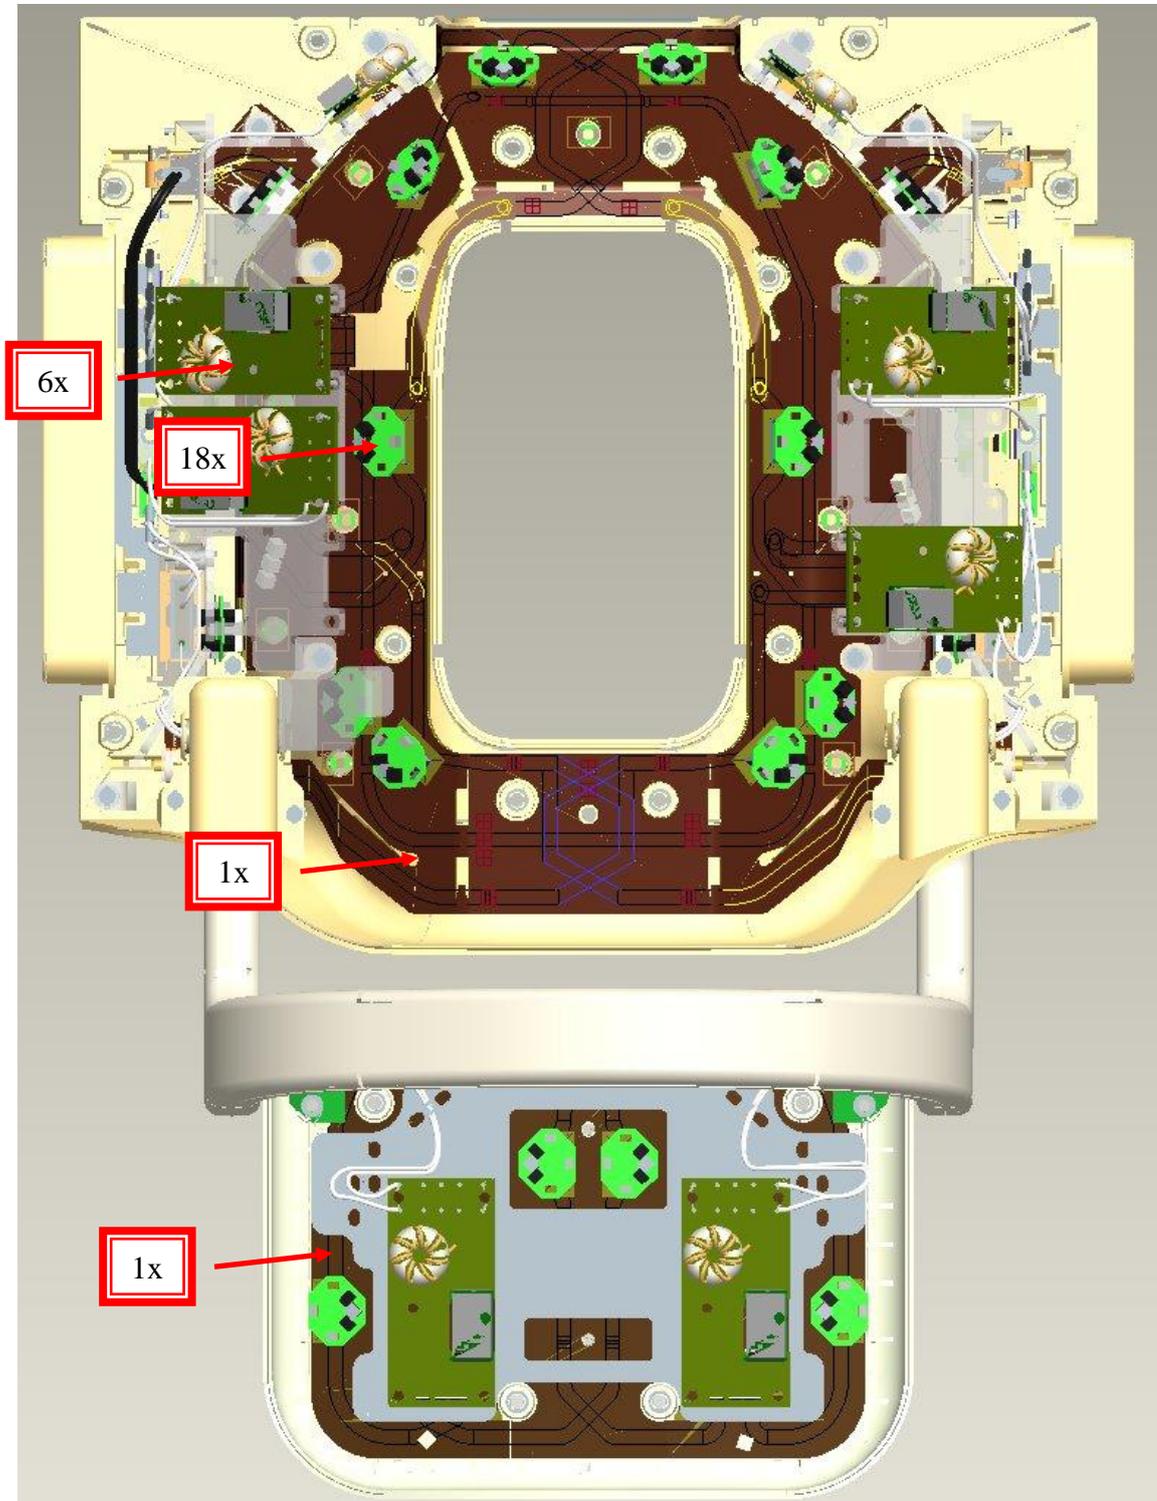


Figure 1, NVC HeadNeck 3.0T pcb locations

| | | | | | |
|---|--|--------------------|----------------|-------------------------------------|-------------------|
| Name: WEEE NVC HeadNeck 3.0T | | 12NC: DMR152840 | | Version: 00 Doc.Date: 2012-07-31 | |
| Author: | | Pag.: 2 of 4 | Group No: 5790 | Section: - | Status: see Agile |
| © PHILIPS MEDICAL SYSTEMS NEDERLAND BV, BEST 2012 | | | | Template version 2. | |

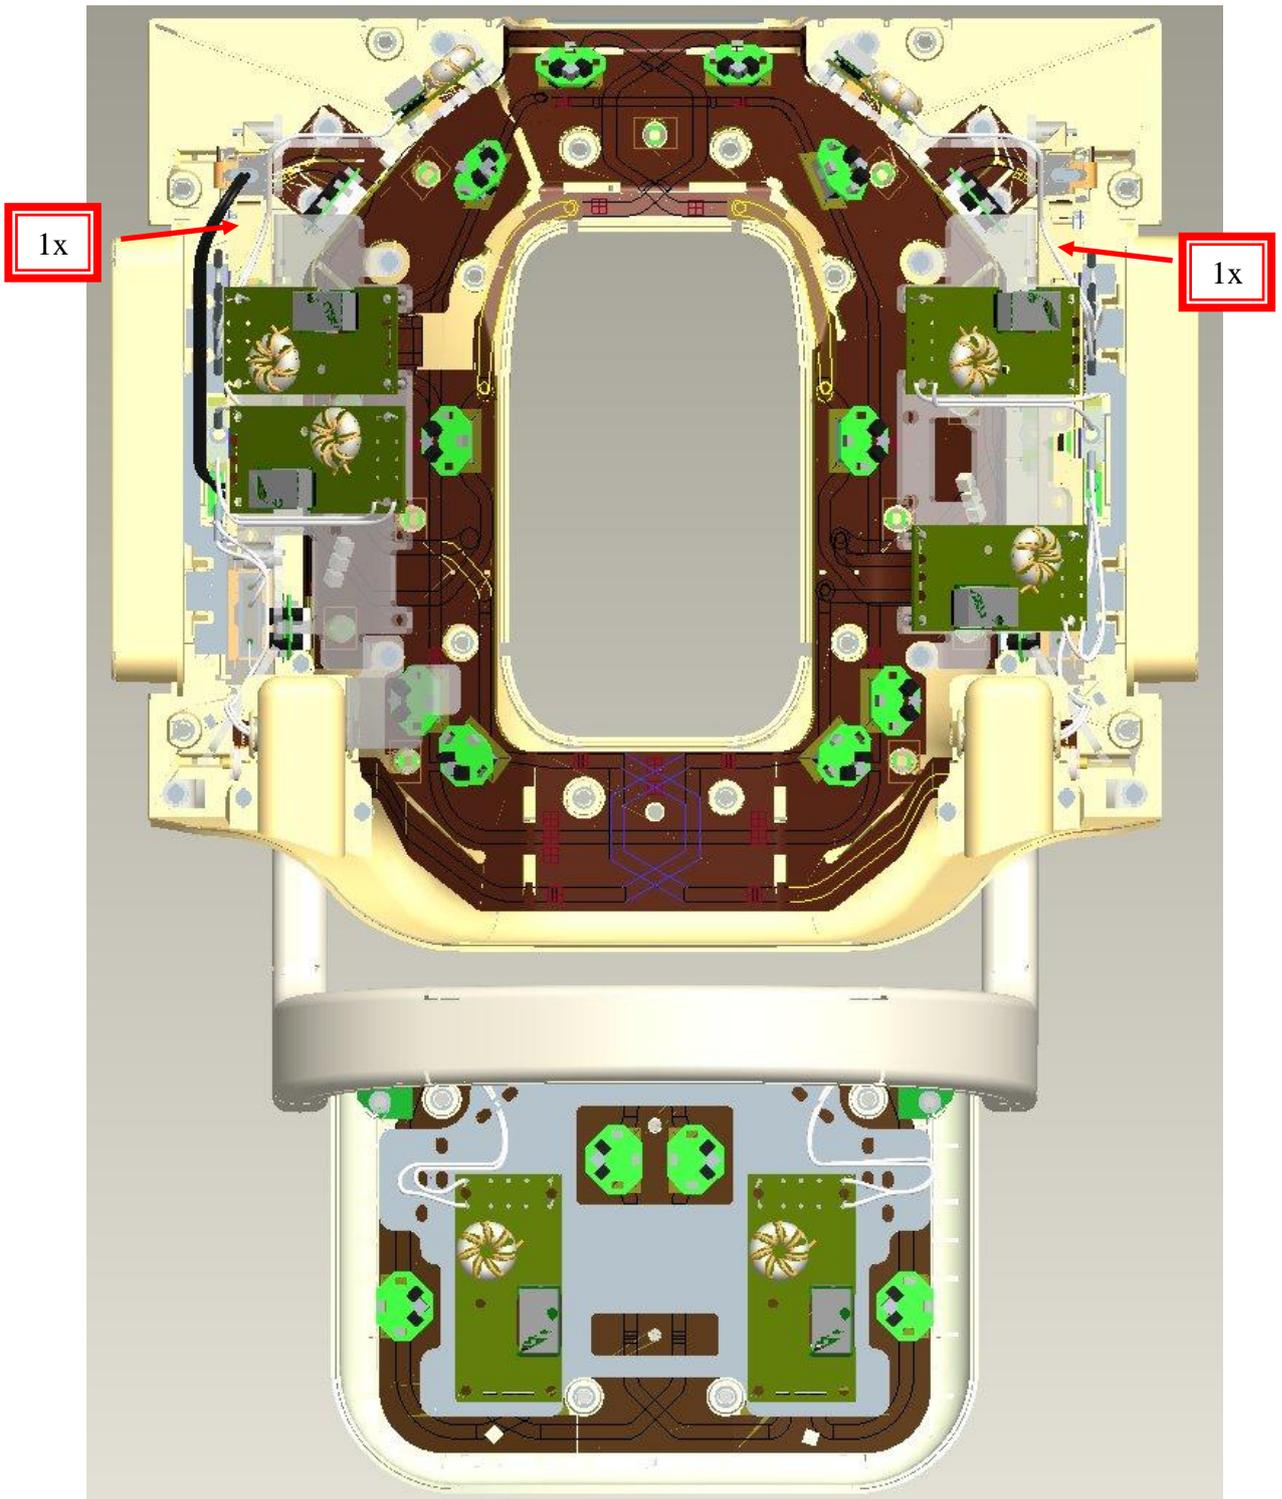


Figure 2, NVC HeadNeck 3.0T RXE locations

| | | | | | |
|---|--|--------------------|----------------|-------------------------------------|-------------------|
| Name: WEEE NVC HeadNeck 3.0T | | 12NC: DMR152840 | | Version: 00 Doc.Date: 2012-07-31 | |
| Author: | | Pag.: 3 of 4 | Group No: 5790 | Section: - | Status: see Agile |
| © PHILIPS MEDICAL SYSTEMS NEDERLAND BV, BEST 2012 | | | | Template version 2. | |

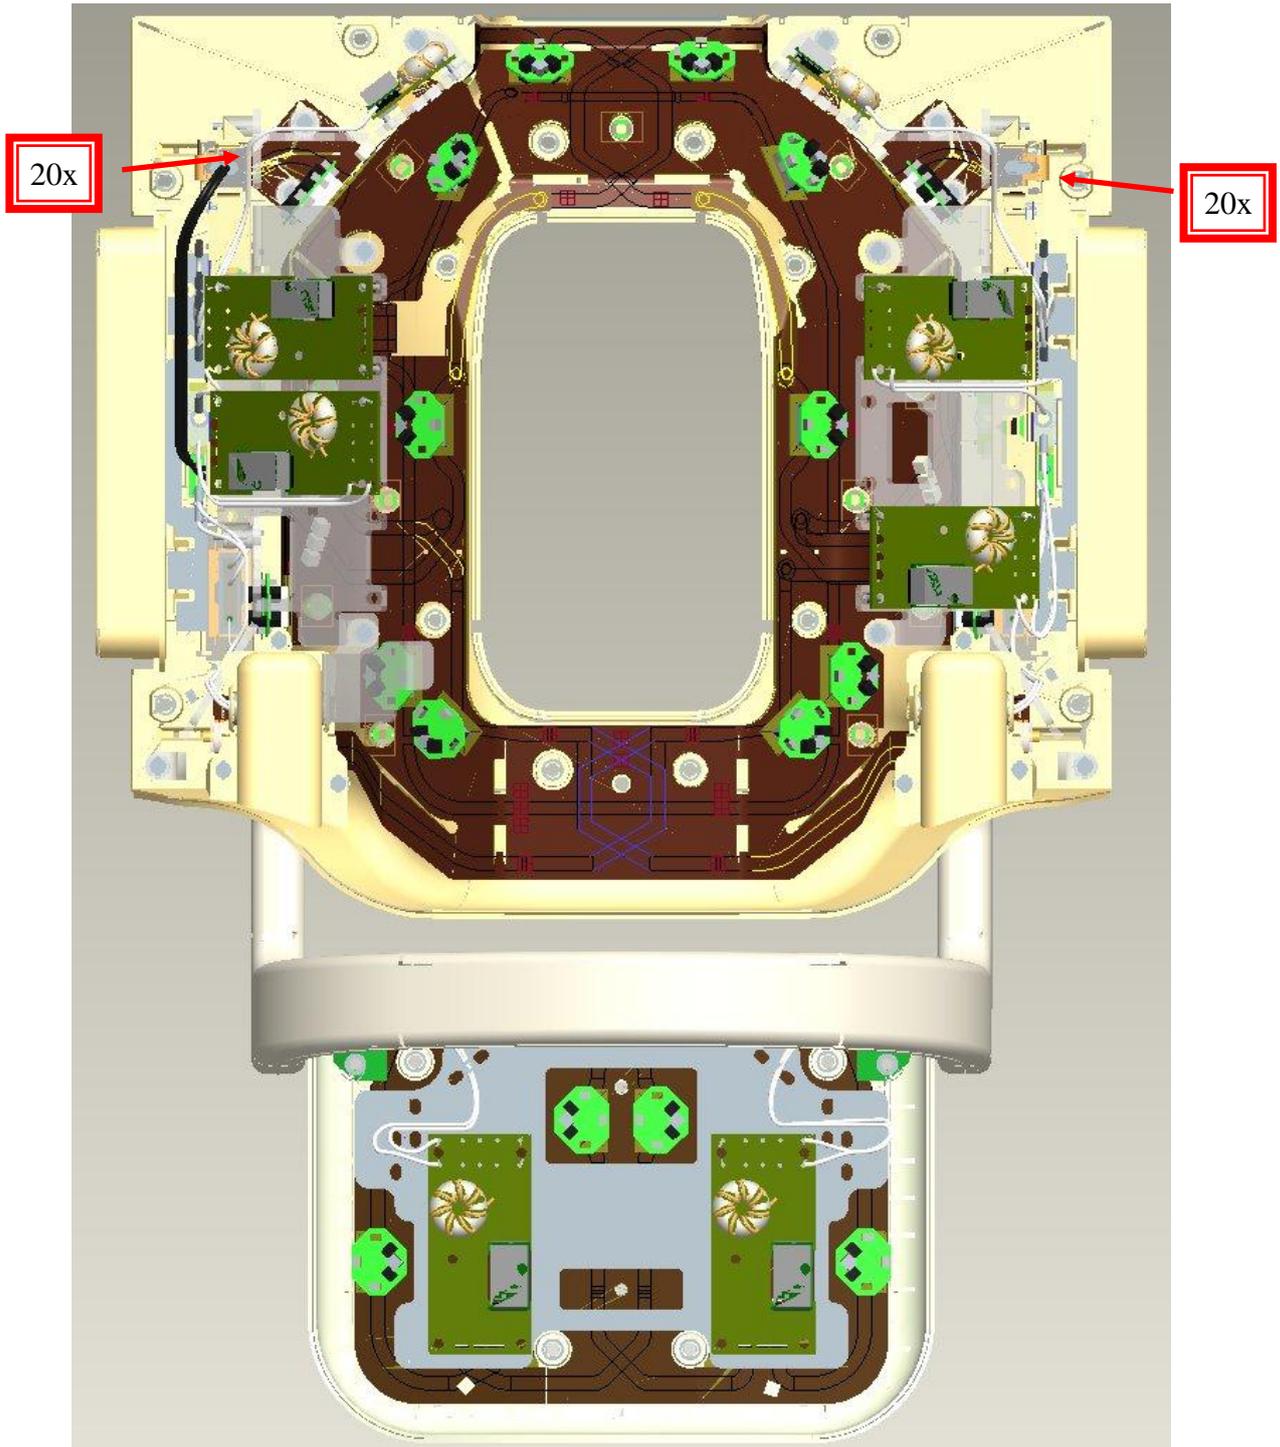


Figure 3, Connector (multiple locations), NVC HeadNeck 3.0T

| | | | | |
|---|--|---------------------------|-------------------------------------|------------|
| Name: WEEE NVC HeadNeck 3.0T | | 12NC: DMR152840 | Version: 00 Doc.Date: 2012-07-31 | |
| Author: | | Pag.: 4 of 4 | Group No: 5790 | Section: - |
| © PHILIPS MEDICAL SYSTEMS NEDERLAND BV, BEST 2012 | | | Status: see Agile | |
| | | | Template version 2. | |