PHILIPS
MEDICAL
SYSTEMS


Product Recycling Passport


QAF90163verA ECO 5-12374 SIGNATURE/DATE: EDMS Page 1 of 8

Product name: T		Tidal V	Tidal Wave		
Identification code(s)		Models 610, 615, 710, 715			
Total weight (in	Kg)	.86 Kg	.86 Kg (Model 715 with NiMH battery option)		
D 1 /	NT				
Producer/	Name o	company:	Respironics Novametrix, LLC		
Manufacturer	Address: Zip code:		5 Technology Drive Wallingford CT		
			06492		
	Country:		United States of America		

Items:	Location		
Disinfect device prior to handling	Figures 1 – 4, 10		
Items: None	Location N/A		
Type:	Location		
AA Lithium Batteries (x7) Optional NiMH Battery (x1) Optional 3 Volt Lithium Battery (615/710/715 Only) 3 Volt Lithium Battery (610 Only)	Figure 5, Location 1 Figure 5, Location 2 Figure 7, Location 2 Figure 7, Location 3		
Substances: PCB - Main board (lead solder) PCB - CO2 Sensor Board (lead solder) PCB - LCD Display Board (lead solder) PCB - Base Station Main Board (lead solder) Power Supply (lead solder)	Location Figure 7, Location 1 Figure 8, Location 1 Figure 9, Location 1 Figure 11, Location 1 Figure 12, Location 1		
	Type: AA Lithium Batteries (x7) Optional NiMH Battery (x1) Optional 3 Volt Lithium Battery (615/710/715 Only) 3 Volt Lithium Battery (610 Only) Substances: PCB - Main board (lead solder) PCB - CO2 Sensor Board (lead solder) PCB - Base Station Main Board (lead solder) PCB - Base Station Main Board (lead solder)		

Passport Number	Version	Author	ECO	Signature/Date
1016112MC5	А	Patrick Freeman	5-13117	EDMS

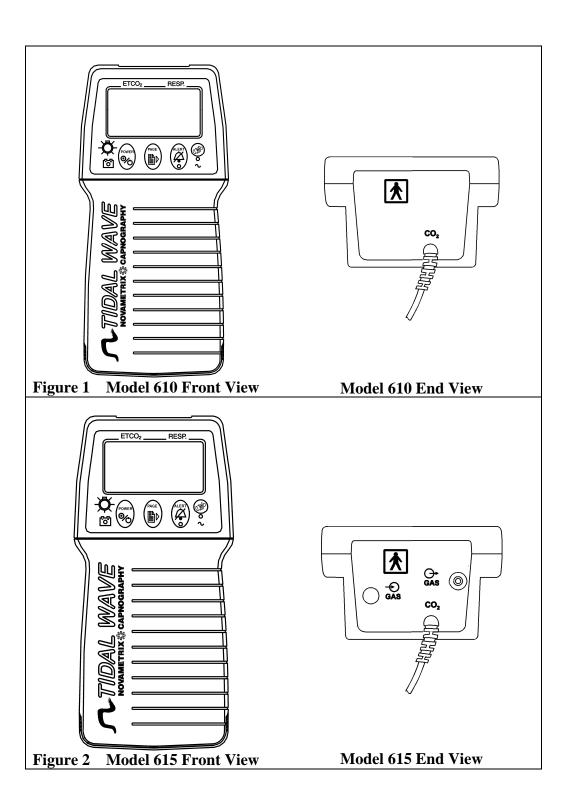

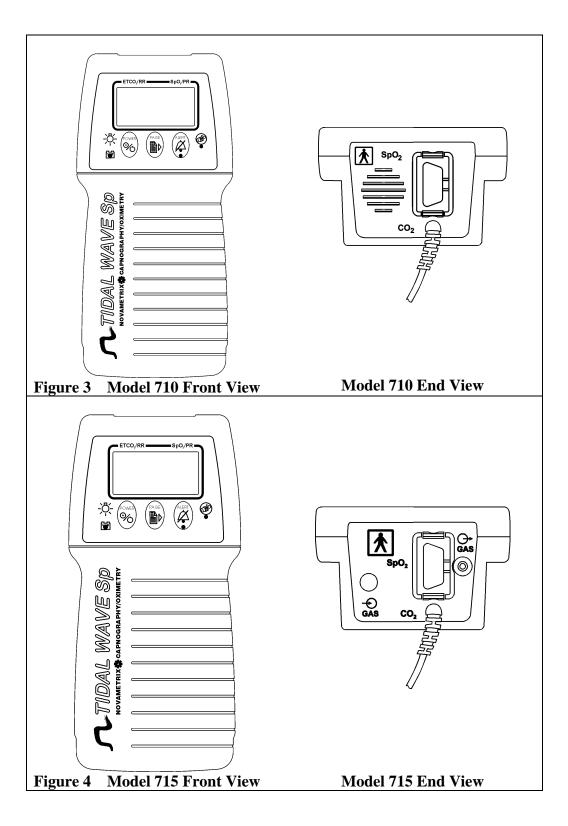


PHILIPS MEDICAL SYSTEMS

Product Recycling Passport

QAF90163verA ECO 5-12374 SIGNATURE/DATE: EDMS

SIGNATURE/DATE: EDMS
Page 4 of 8

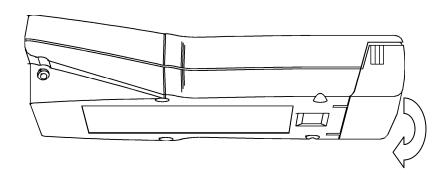

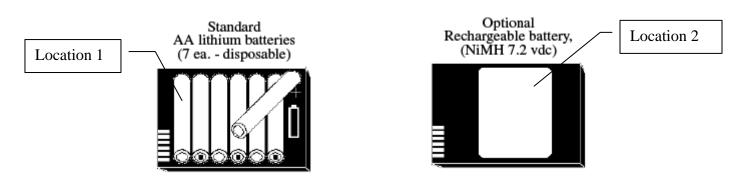


Figure 5 Battery Location and Options

QAF90163verA ECO 5-12374 SIGNATURE/DATE: EDMS

Page 5 of 8

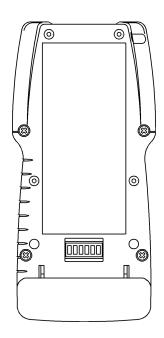


Figure 6

Printed copies are uncontrolled

Rear Panel (all models)

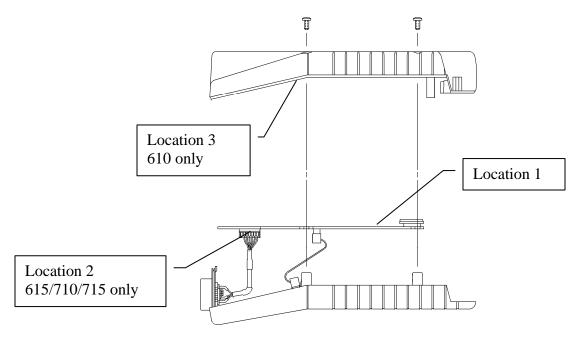


Figure 7

Side view

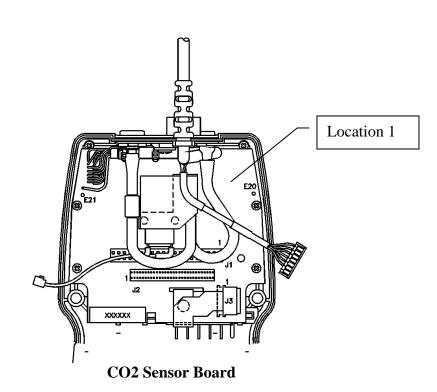


Figure 8

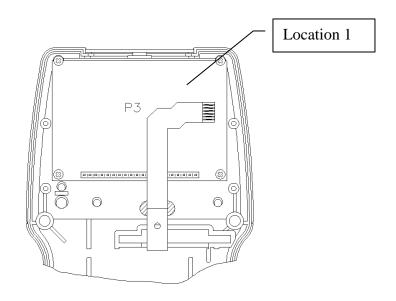


Figure 9

LCD Display Board

Printed copies are uncontrolled

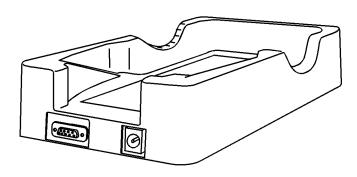
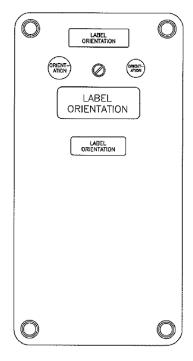


Figure 10 Base Station



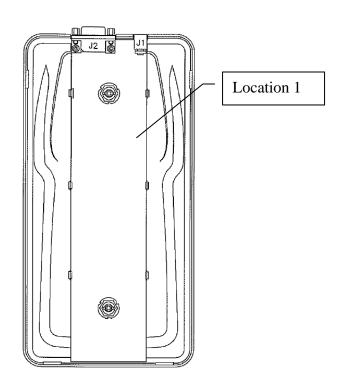


Figure 11 Bottom

PHILIPS
MEDICAL
SYSTEMS

Product Recycling Passport

QAF90163verA ECO 5-12374 SIGNATURE/DATE: EDMS

SIGNATURE/DATE: EDMS
Page 8 of 8

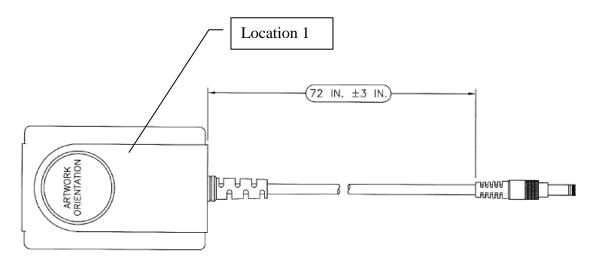


Figure 12

Power Supply (Typical)