Philips Ultrasound and Monitoring

SureSigns VS2i/VS2+ Recycling Passport

Notice

UNCONTROLLED IN PRINTED FORM UNLESS STAMPED IN RED

Document Ownership

The document owner is listed below:

Function	Title
Regulatory System Department	Regulatory Engineer

Revision Summary

The current document revision is described below:

Rev.	Change Order #	Change Summary	
A	See eDMR	As Issued	

Rev. A Document Number: A-863275-90007-1

Title: SureSigns VS2i/VS2+ (863275-863279 inclusive) Recycling Passport

Fig. 1. Page 1. Pag

Product name	:		
	SureSig	gns VS2i/VS2+	
Identification cod	e(s) (Model	(Model) SureSigns VS2i/VS2+	
(Refe		Reference num) 863275, 863276, 863277/863278, 863279	
		(including battery)	
Producer/ Manufacturer	Name company:	Philips Medical Systems	
	Address:	3000 Minuteman Road, Andover MA	
	Zip code:	01810	
	Country:	USA	

Items:	Location
Warning: Before you attempt to open or disassemble the monitor, disconnect the AC power from the monitor and remove the battery. Remove any cables from the measurement modules, and the nurse call and network connections.	Figure 1, 2, 3, 4
N/A	Location
Type:	Location
Lithium Ion battery	Figure 4
Substances:	Location
Tin lead solder on the PCB boards	Figure 14
	Warning: Before you attempt to open or disassemble the monitor, disconnect the AC power from the monitor and remove the battery. Remove any cables from the measurement modules, and the nurse call and network connections. Items: N/A Type: Lithium Ion battery Substances:



AC Power cord connector

Figure 1 – AC Power - disconnect

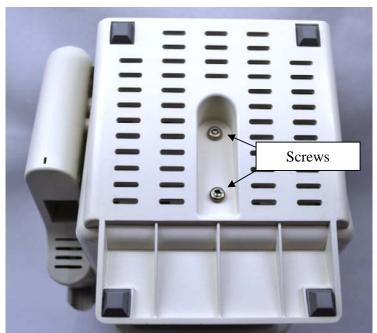


Figure 2 - If your monitor has a tabletop base, remove it by removing the two Torx T20 screws from the bottom of the base.

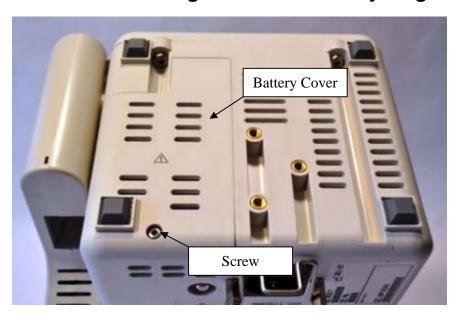


Figure 3 - Remove the Torx T10 screw from the battery cover on the bottom of the monitor.



Figure 4 - Disconnect the battery cable from the connector and remove the battery from the monitor

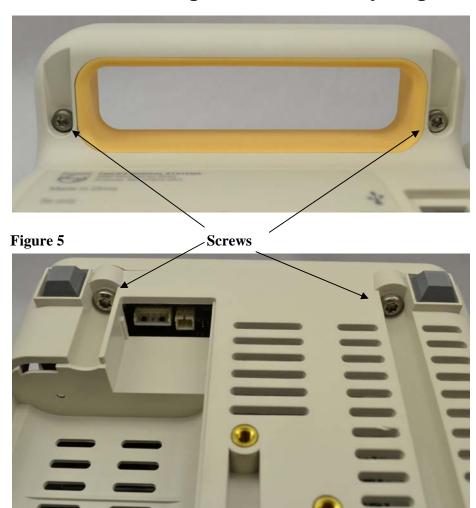


Figure 6

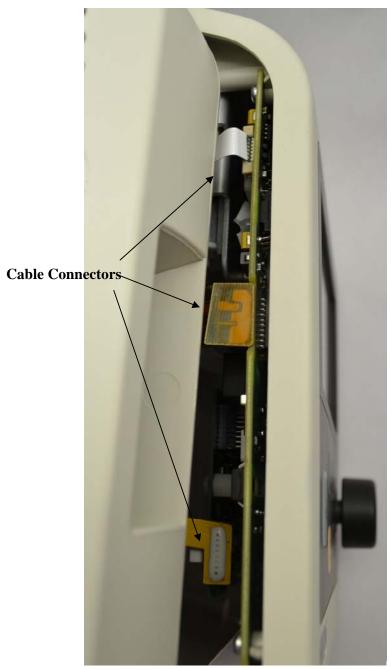


Figure 7



Figure 8

Cable

NBP

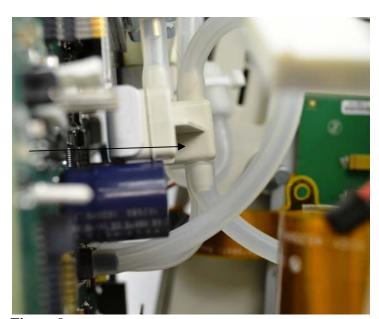


Figure 9

