


Product name:	Transcutaneous O2/CO2 Monitor and Gas Calibrator	
Identification code(s)	Model 860 (monitor) and Model 868 (calibrator)	
Total weight (in Kg)	3.6 Kg (860), 1.4 Kg (868)	
Producer/ Manufacturer	Name company:	Respironics California, Inc.
	Address:	2271 Cosmos Court, CA
	Zip code:	92011
	Country:	United States of America

Recycle Info	Items:	Location
Special attention 	Disinfect device prior to handling	Figures 1 and 4
Fluids / Gases 	Items:	Location
	High Point Calibration Gas (10% CO ₂ , 12% O ₂ , Bal N ₂)	Figure 5, Location 1
	Low Point Calibration Gas (5% CO ₂ , 0% O ₂ , Bal N ₂)	Figure 5, Location 2
Batteries 	Type:	Location
	Lead Acid Battery	Figure 3, Location 5
To be Removed		
Hazardous 	Substances:	Location
	PCB - Main Board (Lead Solder)	Figure 3, Location 1
	PCB - Front End Board (Lead Solder)	Figure 3, Location 2
	PCB - Power supply board (Lead Solder)	Figure 3, Location 3
	PCB - Display board (Lead Solder)	Figure 3, Location 4
	Mercury - Florescent tube backlight contains mercury	Figure 3, Location 4
	PCB - Valve Control Board (Lead Solder)	Figure 6, Location 1
To be Removed		

Passport Number	Version	Author	ECO	Signature/Date
1015316MC6	A	Patrick Freeman	5-14745	EDMS

Figure 1 Model 860

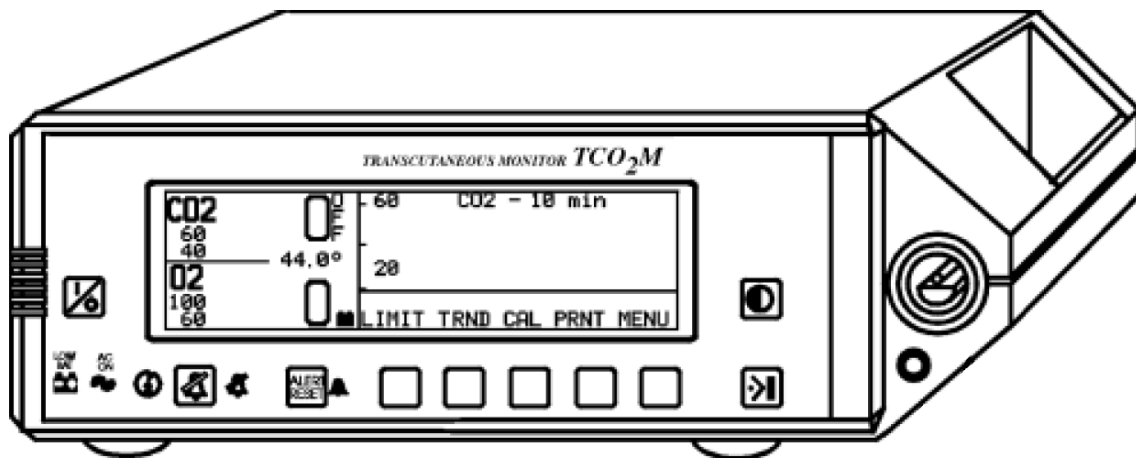


Figure 2 Model 860 Bottom View

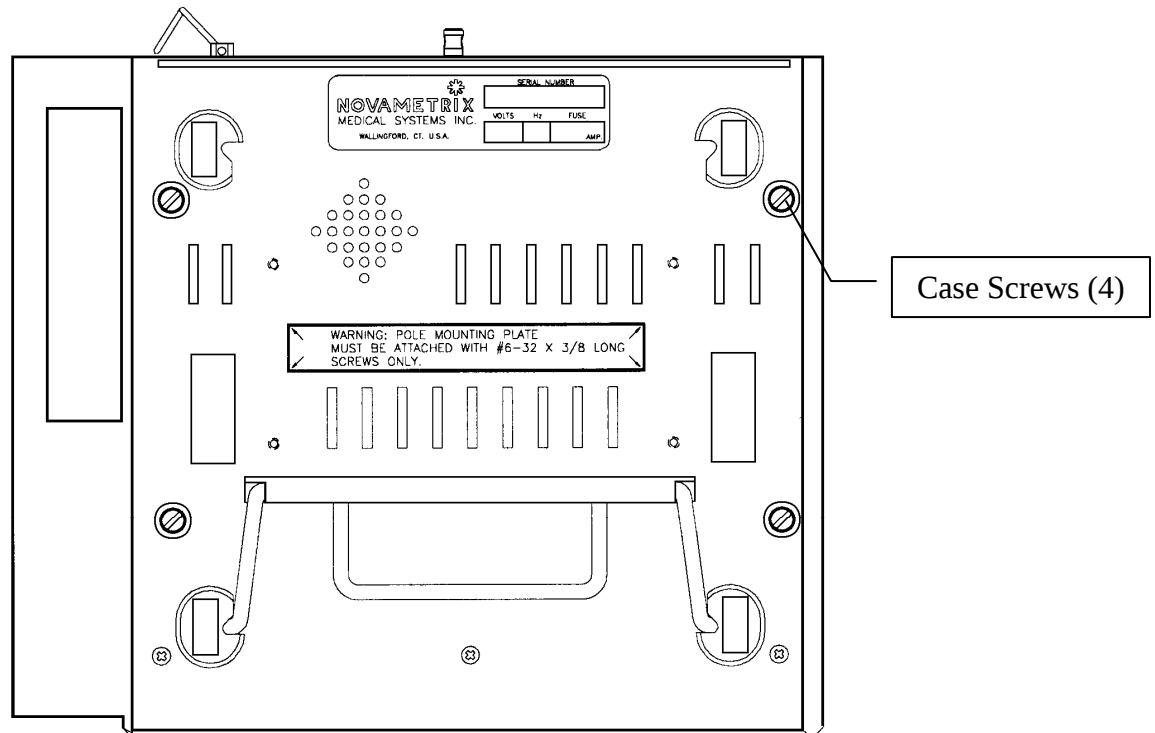


Figure 3 Model 860 Exploded View

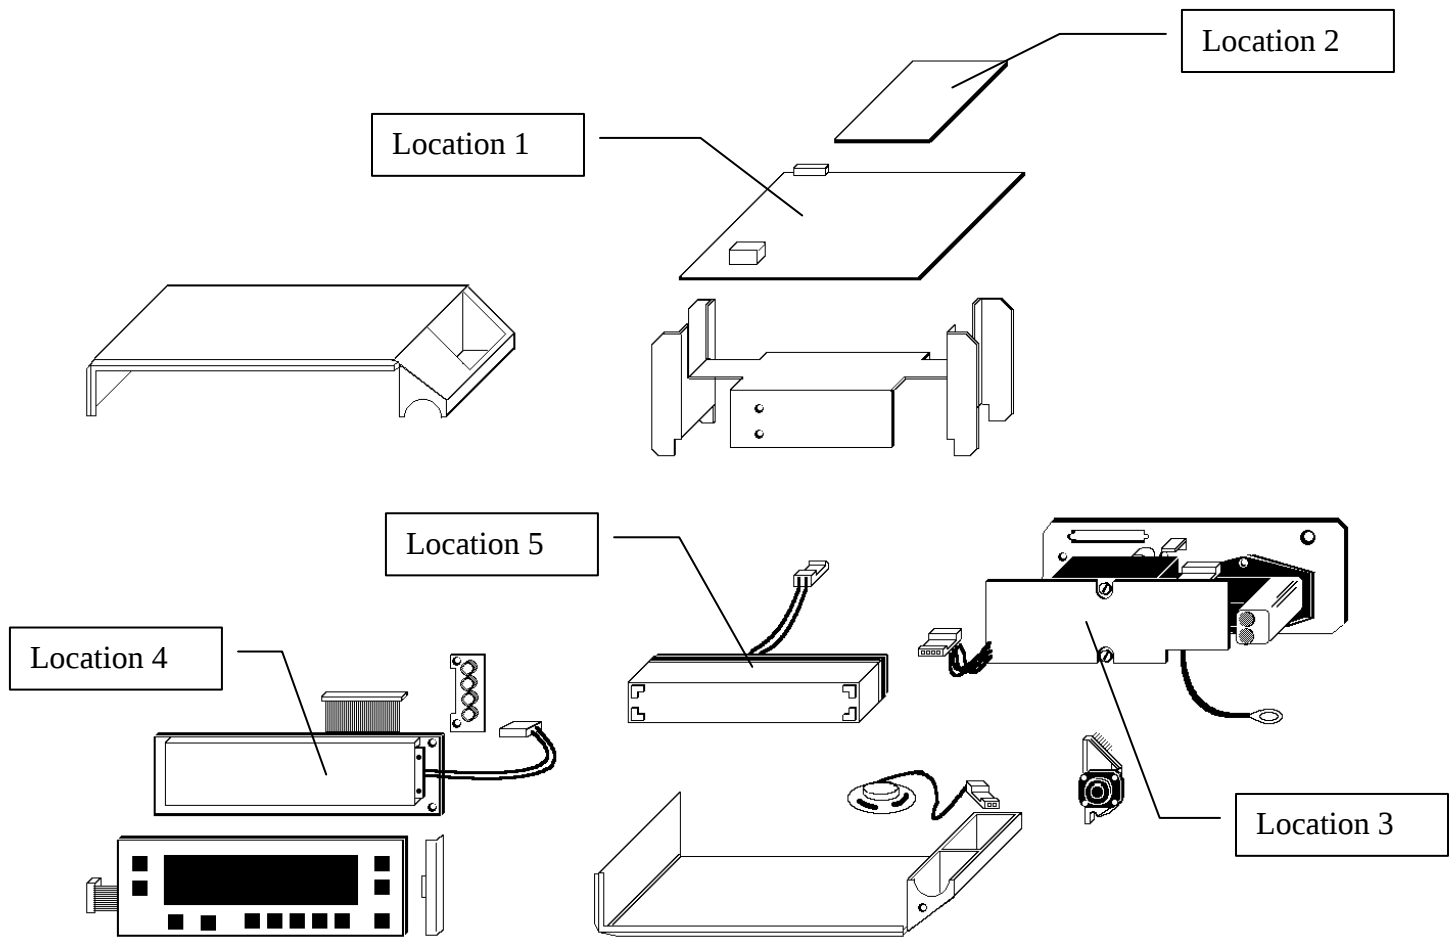


Figure 4 Model 868 Calibrator

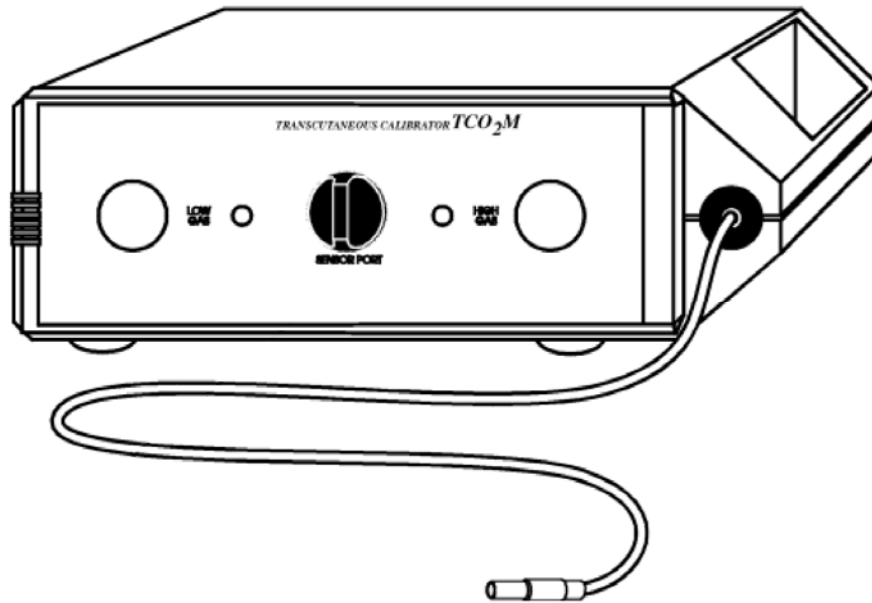


Figure 5 Model 868 Calibrator Rear View

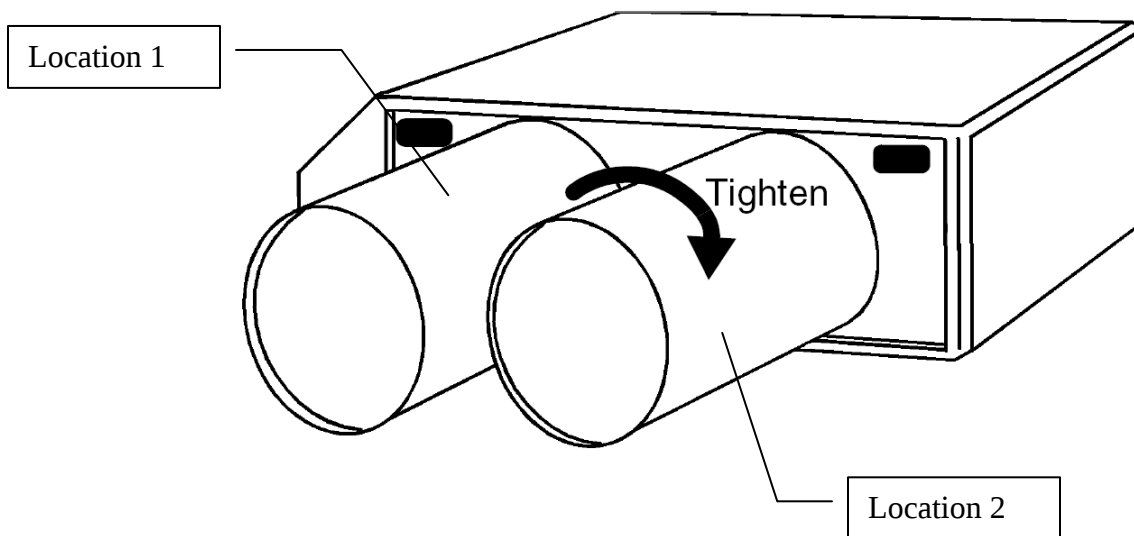


Figure 6 Model 868 Internal View

